



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 1 of 105

1. Introduction

This document reports on the WARM FUNCTIONAL TESTS carried out on the SPIRE Flight Instrument Model in the FM IST test campaign to verify the correct functioning of each of its subsystems before cool down. The Herschel cryostat chamber was in the horizontal configuration (+Y axis pointing upwards) at ambient pressure and temperature. This configuration was necessary in order to perform all the tests which involve unlatching or moving the SMEC. All these tests were performed on 23rd October 2007.

1.1 Scope

To judge the success or failure of a warm functional test by checking that:

- The telecommand sequence generated for a particular functional test is correctly received and executed on board by the SPIRE DPU.
- No error/event reports or command failures are generated during the execution of these commands.
- Telemetry is generated by the instrument as a result of telemetry requests to its different subunits.
- Particular telemetry parameters for each functional test change in an expected manner.
- Success criterion/criteria (specified in this document) is/are met.

1.2 Reference Documents

Ref	Document	Name	Version/Issue Nb.
RD01	SPIRE-RAL-DOC-001652	SPIRE Functional Tests Specification	Issue 1.4
RD02	SPIRE-RAL-DOC-001630	SPIRE EGSE-ILT Start-Up Procedures	Issue 0.7
RD03	SPIRE-RAL-PRC-002222	DRCU Switch ON Procedure	Issue 1.0
RD04	SPIRE-RAL-PRJ-001078	SPIRE Data ICD	Issue 2.1
RD05	Sap-SPIRE-CCa-076-02	DRCU/DPU Interface Control Document	Issue 1.2
RD06	LAM.PJT.SPI.NOT.011011	MCU/DPU Command List ICD	Issue 5.0
RD07	SPIRE-IFS-PRJ-001391	SPIRE OBS User Manual	Issue 2.2
RD08	SPIRE-IFS-PRJ-000650	SPIRE DPU Interface Control Document	Issue 1.1
RD09	SPIRE-RAL-PRC-002841	SPIRE I-EGSE Setup Procedure	Issue 2.1

1.3 Change Record

Document	Change date	Changes
Issue 1.0	23 th Oct 2007	First version
Issue 1.1	19 th Apr 2007	Comments for FUNC-DCU-13-PHOT and FUNC-DCU-13-SPEC updated. Typos corrected.



TABLE OF CONTENTS

1. Introduction..... 1
 1.1 Scope..... 1
 1.2 Reference Documents..... 1
 1.3 Change Record..... 1
2. Functional Tests Configuration..... 4
 2.1 SPIRE Instrument Configuration (PRIME)..... 4
 2.2 Software Configuration (PRIME)..... 4
 2.3 EGSE Configuration Checks..... 4
3. Test procedure..... 6
 3.1 General Pass/Fail Criteria..... 6
4. Detailed Test Results on PRIME instrument..... 7
 4.1 FUNC-SCU-01: SCU Science Generation Check..... 7
 4.2 FUNC-SCU-03: SCU DC Thermometry Check..... 9
 4.3 FUNC-SCU-06: SCU AC Thermometry Check..... 11
 4.4 FUNC-SCU-02: SCU Nominal Science Contents Check..... 13
 4.5 FUNC-SCU-04: Photometer Calibration Check..... 15
 4.6 FUNC-SCU-05: Spectrometer Calibration Check..... 16
 4.7 FUNC-SCU-07: SCU Cooler Heater Check..... 17
 4.8 FUNC-SCU-08: SCU Test Pattern Check..... 19
 4.9 FUNC-MCU-01: MCU Boot Check..... 21
 4.10 FUNC-MCU-02: MCU Nominal Frame Generation Check..... 23
 4.11 FUNC-MCU-03: MCU Nominal Science Contents Check..... 25
 4.12 FUNC-MCU-04: MCU Test Pattern Check..... 27
 4.13 FUNC-BSM-01: BSM Chop/Jiggle Sensor Check..... 29
 4.14 FUNC-BSM-02C: BSM Chop Sensor Polarity Check..... 31
 4.15 FUNC-BSM-02J: BSM Jiggle Sensor Polarity Check..... 33
 4.16 FUNC-BSM-03: BSM Open Loop Dynamics Check..... 35
 4.17 FUNC-BSM-05A: BSM Open Loop Chop Test..... 38
 4.18 FUNC-BSM-05B: BSM Closed Loop Chop Test..... 41
 4.19 FUNC-BSM-06: BSM Operational Mode Check..... 43
 4.20 FUNC-DCU-01: DCU Nominal Science Packet Generation Check..... 46
 4.21 FUNC-DCU-02: DCU High Speed Link Check..... 50
 4.22 FUNC-DCU-03: DCU Test Pattern Check..... 52
 4.23 FUNC-DCU-04-PHOT: Photometer LIAs Check..... 54
 4.24 FUNC-DCU-11-PHOT: Photometer BDAs Switch ON Check..... 57
 4.25 FUNC-DCU-13-PHOT: Photometer BDAs Integrity Check..... 59
 4.26 FUNC-DCU-14-PHOT: Photometer BDAs Noise Check..... 62
 4.27 FUNC-DCU-04-SPEC: Spectrometer LIAs Check..... 64
 4.28 FUNC-DCU-11-SPEC: Spectrometer BDAs Switch On Check..... 66
 4.29 FUNC-DCU-13-SPEC: Spectrometer BDAs Integrity Check..... 68
 4.30 FUNC-DCU-14-SPEC: Spectrometer BDAs Noise Check..... 70
 4.31 FUNC-SMEC-01: SMEC Encoder and LVDT Check..... 72
 4.32 FUNC-SMEC-03: SMEC Encoder Levels Check..... 74
 4.33 FUNC-SMEC-02A: SMEC Open Launch Latch..... 75
 4.34 FUNC-SMEC-04A: SMEC Open Loop Position Check..... 77
 4.35 FUNC-SMEC-09: SMEC Open Loop Scan Check..... 79
 4.36 FUNC-SMEC-07: SMEC Closed Loop Scan Test..... 85
 4.37 FUNC-SMEC-02B: SMEC Close Launch Latch..... 87



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	3 of 105

5.	Annexe 1 (DCU Test Pattern Data)	91
6.	Annexe 2 (Results of Load Curves).....	97



2. Functional Tests Configuration

2.1 SPIRE Instrument Configuration (PRIME)

SPIRE FPU:

- FPU in tank.
- Cryo-harness connected to FPU
- DRCU to Cryostat harnesses connected (Grounding pins not connected)
- DRCU-DPU Harness connected
- Cryostat open

2.2 Software Configuration (PRIME)

The current EGSE software configuration for the PRIME side tests:

EGSE component	Version/Build number	Comment
SCOS2000	SCOS2.3e Patch 5	SCOS archives IST_FM1 under /data/SPIRE/hfiles and /data/SPIRE/TMD SCOS MIB is FM_2.2.G6_PR_
CDMS Simulator	v2.5	NA
HCSS	#1206	
QLA	3.3 Build #555	
QLA scripts	Latest CVS versions	
Test Control scripts		CCS Handler scripts CVS v1.4
CUS Scripts		Mission config fm_ist_wft_config_prime4
Versant	7.0.0.1	
TFCS		NA
TFTS		NA

2.3 EGSE Configuration Checks

To check for the success of failure of a functional test, the real time telemetry of the instrument has to be monitored. The following applications must be running to do so. Before the test sequence starts, make the following checks:

Workstation	EGSE component	Status	Check	Comments
hspireegse	EGSE Router	Started	✓	Running
hspireegse	EGSE Gateway	Started	✓	Running
hspireegse	Pipe GW	Started	✓	Running
spireqla	Telemetry Ingestion	Started	✓	Running
spireqla	Packet Display	Started	✓	Running



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	5 of 105

spireqla	CCS Handler Server	Started	✓	Running
spires2k	SCOS2000	Started	✓	Running
spireqla	QLA	Started	✓	Running

The following checks were performed to verify the correct initial instrument configuration for the tests.

Step#	Action	Comments	Check
1.	In SCOS open DPU_AND_OBS_PARAMETERS display Check if: TM2N is incrementing by one @1Hz. TM1N is incrementing by one @0.5Hz. - If they are, go to step 5. - If they are not, go to step 2.	Both TM1N and TM2N are incrementing at their nominal rates. Will go to step 5. DPUM15V=-15.88V DPUTEMP = 299.06K	✓
2.	In SCOS open SCU PARAMETERS display - If SCUP5V/P9V/M9V are jittering and BIAS_PARAMETERS display - If BIASTEMP show ambient temperature, the DRCU is ON.Go to step 6. - If DRCU is not ON, refer to RD03 on how to start up the DRCU.	ALL SCU VOLTAGES LOOKING GOOD. SCUP5V = 5.24V SCUP9V =9.08V SCUM9V = -9.08V ALL BIAS VOLTAGES LOOKING GOOD. BIASP5V = 5.18V BIASP9V = 8.99V BIASM9V= -9.05V BIASTEMP=293.8K	✓
3.	In SCOS open DPU_AND_OBS_PARAMETERS display and check that the MODE housekeeping parameter is DRCU_ON.	MODE (RAW)= 0x100 MODE (ENG) = DRCU_ON	✓

Table 1. Initial configuration check



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	6 of 105

3. Test procedure

The following two sections describe general pass/fail criteria (Section 3.1), the general test procedure layout (Section 3.1) and the detailed procedure for each functional test (Section 3.2).

3.1 General Pass/Fail Criteria

The general criterion for declaring a single test failed is the repeated failure of 2 consecutive runs of this test. In that case the functional test procedure should be aborted and the overall functional testing declared FAILED.

In the case of a 'first run' failure followed by a successful execution a third run of the same test should be performed and in the unlikely event of this third run being a failure the test procedure should be also aborted and the overall functional testing declared FAILED, as this would imply a not reliable operability of the instrument.

As a general remark ANY failure should be closely analyzed.



4. Detailed Test Results on PRIME instrument.

The following is a detailed (test by test) procedure including the steps performed on each test and the results obtained.

Step#	Action	Comments
0	Open SCU PARAMETERS display on SCOS Alpha Numeric Displays.	

4.1 FUNC-SCU-01: SCU Science Generation Check

Test Id:	FUNC-SCU-01: SCU Science Generation Check												
Initial Configuration:	DRCU_ON												
Final Configuration:	DRCU_ON												
Success Criteria:	<p>Test passed if :</p> <ol style="list-style-type: none"> Two SCU Nominal Science Report telemetry packets are received on QLA with the following characteristics: <table border="1" style="margin-left: 40px;"> <thead> <tr> <th>APID</th> <th>Type</th> <th>Subtype</th> <th>SID</th> <th>FrameID</th> <th>Frame length</th> </tr> </thead> <tbody> <tr> <td>0x508</td> <td>21</td> <td>1</td> <td>0xA20</td> <td>0x20</td> <td>0x1E</td> </tr> </tbody> </table> <ol style="list-style-type: none"> The frame time difference between consecutive SCU frames within these packets corresponds to the sampling rate. Nominal SCU sampling rate is 80Hz → Δt = 12.5 ms The SPIRE HK parameter SCUFRAMECNT increments by 31. No events are generated during the frame generation. <p>QLA to give go ahead.</p>	APID	Type	Subtype	SID	FrameID	Frame length	0x508	21	1	0xA20	0x20	0x1E
APID	Type	Subtype	SID	FrameID	Frame length								
0x508	21	1	0xA20	0x20	0x1E								

Test Procedure:

Step#	Action	Comments
1	Write the initial value of SCUFRAMECNT parameter located in SCU PARAMETERS display and the initial value of TM1N located in DPU_AND-OBS_PARAMETERS display.	SCUFRAMECNT = 0
2	Run QLA script FUNC-SCU-01.py on QLA console.	
3	Run FUNC-SCU-01 test procedure from the CCS	
4	Write the final value of SCUFRAMECNT and TM1N.	SCUFRAMECNT = 31
5	Contingency: If test fails repeat steps 1 to 4.	

Test Log:



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 8 of 105

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SCU-01	SCUFRAMECNT TM5N	n/ n+ 31 0x3FFF/1	0/ 31 0x3FFF/1	31	Success

Start time: 09:42
OBSID: 0xb00002b8

CUS Input Default Parameters:
 scuframes = 0x1F – Number of SCU frames to generate

Comments:
QLA produced QLA-SCU-01_B00002B8.txt file:

```
*****
SCU: OBSID = B00002B8, BBTYP E = 0x8000, APID = 0x508, SID = 0xa20

Parameter      Initial      Final      Increment Expect Incre. Packet Chars.
-----
SCUFRAMECNT    0            31         31          31          Packet type = 0x15
TM5N           16383        1          2            2          subtype = 0x1
FrameTime      12.4960     12.4992
Frame Len      0x1E

STATISTICS ON TIME BETWEEN RECEPTION OF 2 CONSECUTIVE FRAMES:
mean = 12.49803 ms
sigma = 0.00156 ms
```




SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	9 of 105

4.2 FUNC-SCU-03: SCU DC Thermometry Check

Test Id:	FUNC-SCU-03: SCU DC Thermometry Check
Initial Configuration:	DRCU_ON
Final Configuration:	DRCU_ON + DC thermometry ON
Success Criteria:	<p>Test passed if all FPU DC thermometry sensors show temperature values indicating a correct functioning of the sensor, not open/short-circuited. If ANY reading is anomalous check RAW sensor reading.</p> <p>Open Circuit Criterion: RAW reading in the range [0, -100]</p> <p>Short Circuit Criterion: RAW reading of -32768</p> <p>Note: For some parameters the calibration curve above 75K has only 2 points, thus the linearly interpolated temperature reading given by SCOS is usually not correct at $T > 75K$.</p>

Test Procedure:

Step#	Action	Comments
1	Run FUNC-SCU-03 test procedure from the CCS	
2	When the test is finished Write the current value of SCUTEMPSTAT and the RAW/converted values of the 16 FPU temperatures located in SCU PARAMETERS display.	
3	Contingency: If test fails execute SCU_OFF procedure from the CCS and repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SCU-03	SCUTEMPSTAT	0/0xFFFF	0/0xFFFF	N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 10 of 105

Start time: 09:44
OBSID:0xb00002b9

CUS Input Default Parameters:

dcparam = 0xFFFF – Switch on all 16 SCU DC thermometry channels

Comments: On SCOS all RAW SCU DC temperatures are 32768 except EMCFILTEMP which is -29822

QLA script produced the file FUNC-SCU-03_B00002B9.txt:

SCU-03 Thermometry Check
OBSID = 0xb00002b9

PUMPHRTEMP	54.11	32768
PUMPHSTEMP	37.26	32768
EVAPHSTMP	36.90	32768
SHUNTTEMP	18.71	32768
EMCFILTMP	286.38	35716
SLOTTEMP	19.72	32768
PLOTEMP	20.33	32768
OPTTEMP	154.06	32768
BAFTEMP	181.37	32768
BSMIFTEMP	98.86	32768
SCAL2TEMP	161.08	32768
SCAL4TEMP	156.52	32768
SCALTEMP	83.34	32768
SMECIFTEMP	137.97	32768
SMECTEMP	26.54	32768
BSMTEMP	12.80	32768



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	11 of 105

4.3 FUNC-SCU-06: SCU AC Thermometry Check

Test Id:	FUNC-SCU-06: SCU AC Thermometry Check
Initial Configuration:	DRCU_ON + DC thermometry ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON
Success Criteria:	Test passed if SUBKSTAT parameter went from 0 to 1. Open Circuit Criterion: RAW reading in the range 0 -100 Short Circuit Criterion: RAW reading of -32768

Test Procedure:

Step#	Action	Comments
1	Run FUNC-SCU-06 test procedure from the CCS.	
2	When the test is finished Write the current value of SUBKSTAT located in SCU PARAMETERS display. Also write down the RAW value of the SUBKTEMP parameter.	
3	Contingency: If test fails : Send manual command: SEND_DRCU_COMMAND Parameter1 = 0xA0860000 Parameter2 = 0 Then repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SCU-06	SUBKSTAT	0/1	0/1	N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 12 of 105

Start time: 09:47

OBSID:0xb00002ba

CUS Input Default Parameters:

acparam = 0x1 – Switch on SCU AC thermometry channel (SUBKTEMP)

Comments: OK

SUBKTEMP:

Before: RAW = 32754

After : RAW = 32746-32747

QLA output file:

SCU-06
Start time @: 23-Oct 09:48:15
End time @: 23-Oct 09:48:30
OBSID: 0xB00002BA

SUBKSTAT:
Start value: 0x0
End value: 0x1

SUBKTEMP
RAW value before: 32756

RAW value after: 32749
Converted after: 271248 mK



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	13 of 105

4.4 FUNC-SCU-02: SCU Nominal Science Contents Check

Test Id:	FUNC-SCU-02: SCU Nominal Science Contents Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON
Success Criteria:	Test passed if : <ol style="list-style-type: none"> 1. Parameters in the SCU Nominal science packets and the same parameters in the Nominal HK packet have similar RAW values to within ± 10 units. 2. The SPIRE HK parameter SCUFRAMECNT located in SCU PARAMETERS display increments by 31. 3. No events are generated during the frame generation. QLA to give the go ahead.

Test Procedure:

Step#	Action	Comments
1	Write the current value of SCUFRAMECNT located in SCU PARAMETERS display.	
2	Run QLA script FUNC-SCU-02.py on QLA console.	
3	Run FUNC-SCU-02 test procedure from the CCS	
4	When the test is finished Write the current value of SCUFRAMECNT.	
5	Contingency: If test fails repeat steps 1 to 4.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SCU-02	SCUFRAMECNT TMSN	n+31/n+62 1/3	31/62 1/3	31	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 14 of 105

Start time: 09:51
OBSID: 0xb00002bb

CUS Input Default Parameters:

scuframes = 0x1F – Number of SCU frames to generate

Comments:

All SCU parameters within the Nominal HK and the Nominal SCU Science Report agree.

QLA produced QLA-SCU-02_B00002BB.txt file:

FUNC-SCU-02 version: 1.5

Housekeeping @ Tue Oct 23 09:52:12 UTC 2007
SCU Science @ Tue Oct 23 09:52:08 UTC 2007

Name	HSK value	SCU value	Equal (within 10 raw units)?
TCHTRV	20.0	21.0	True
PCALCURR	11.0	11.0	True
SCAL4CURR	9.0	11.0	True
SCAL2CURR	12.0	10.0	True
PCALV	9.0	9.0	True
SCAL4V	11.0	12.0	True
SCAL2V	10.0	11.0	True
PUMPHRTEMP	32768.0	32768.0	True
PUMPHSTEMP	32768.0	32768.0	True
EVAPHSTEMP	32768.0	32768.0	True
SHUNTTEMP	32768.0	32768.0	True
EMCFILTEMP	35716.0	35714.0	True
SL0TEMP	32768.0	32768.0	True
PL0TEMP	32768.0	32768.0	True
OPTTEMP	32768.0	32768.0	True
BAFTEMP	32768.0	32768.0	True
BSMIFTEMP	32768.0	32768.0	True
SCAL2TEMP	32768.0	32768.0	True
SCAL4TEMP	32768.0	32768.0	True
SCALTEMP	32768.0	32768.0	True
SMECIFTEMP	32768.0	32768.0	True
SMECTEMP	32768.0	32768.0	True
BSMTEMP	32768.0	32768.0	True
SUBKTEMP	32749.0	32747.0	True



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	15 of 105

4.5 FUNC-SCU-04: Photometer Calibration Check

Test Id:	FUNC-SCU-04: Photometer Calibration Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON
Success Criteria:	<p>Test passed if PCALCURR/PCALV SCU HK parameters show the following values:</p> <ul style="list-style-type: none"> PCALCURR HK parameter which shows the measured PCAL current is ~ 0.1 mA. PCALV HK parameter which shows the measured PCAL voltage is ~ 0.02V

Test Procedure:

Step#	Action	Comments
1	Write the current value of PCALV and PCALCURR located in SCU PARAMETERS display.	
2	Run FUNC-SCU-04 test procedure from the CCS	
3	While the test is running Write the values of PCALV and PCALCURR.	
4	Contingency: If test fails repeat steps 1 to 3.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/During test	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SCU-04	PCALCURR PCALV	0/0.1mA 0/0.02V	0 / 0.1010 mA 0 / 0.0217 V	N/A	Success

Start time: 09:53
OBSID:0xb00002bc

CUS Input Default Parameters:
pcalbias = 0.1mA – PCAL current

Comments:
Test Successful



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	16 of 105

4.6 FUNC-SCU-05: Spectrometer Calibration Check

Test Id:	FUNC-SCU-05: Spectrometer Calibration Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON
Success Criteria:	Test passed if : <ul style="list-style-type: none"> • SCAL2CURR ,SCAL4CURR HK parameters which show the measured current read ~ 0.1 mA • SCAL2V,SCAL4V parameters which show the measured voltage read ~ 0.05V.

Test Procedure

Step#	Action	Comments
1	Write the current value of SCAL2V ,SCAL2CURR,SCAL4V,SCAL4CURR located in SCU PARAMETERS display.	
2	Run FUNC-SCU-05 test procedure from the CCS	
3	While the test is running write the values of SCAL2V ,SCAL2CURR, SCAL4V,SCAL4CURR.	
4	Contingency: If test fails repeat steps 1 to 3.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/During test	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SCU-05	SCAL4CURR SCAL4V SCAL2CURR SCAL2V	0/0.1mA 0/0.05V 0/0.1mA 0/0.05V	0 / 0.1016 mA 0 / 0.0509 V 0 / 0.1014 mA 0 / 0.05 V	N/A	Success

Start time: 09:55
OBSID:0xb00002bd

CUS Input Default Parameters:
 scal4bias = 0.1mA – SCAL4 current
 scal2bias = 0.1mA – SCAL2 current

Comments:
Test Successful



4.7 FUNC-SCU-07: SCU Cooler Heater Check

Test Id:	FUNC-SCU-07: SCU Cooler Heater Check		
Initial Configuration:	DRCU_ON + AC/DC thermometry ON		
Final Configuration:	DRCU_ON + AC/DC thermometry ON		
Success Criteria:	Test passed if during the execution of the test the following SCU HK parameters give correspondent readings of:		
	SCU HK parameter	RAW	Converted
	SPHSV	~12715	~323mV
	EVHSV	~12715	~323mV
	SPHTRV	~14390	~ 8 V

Test Procedure:

Step#	Action	Comments
1	Run FUNC-SCU-07 test procedure from the CCS.	Pending
2	While the test is running Write the values of current values of SPHSV, EVHSV, SPHTRV located in SCU PARAMETERS display. (RAW and CONVERTED)	
3	Contingency: If test fails repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/During test	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SCU-07	SPHSV EVHSV SPHTRV	0/ ~ 323 mV 0/ ~ 323 mV 0/ ~ 8 V	0.1554 / 324.49mV 0.1554 / 324.28 mV 0.0042 / 8.8552 V	N/A	Success

Start time: 09:56
OBSID:0xb00002be

CUS Input Default Parameters:

evaphs = 0.804mA – Evaporator heat switch current
pumphs = 0.804mA – Sorption pump heat switch current
pumpht = 21.85mA – Sorption pump heater current

Comments:

Test Successful



4.8 FUNC-SCU-08: SCU Test Pattern Check

Test Id:	FUNC-SCU-08: SCU Test Pattern Check												
Initial Configuration:	DRCU_ON + AC/DC thermometry ON												
Final Configuration:	DRCU_ON + AC/DC thermometry ON												
Success Criteria:	<p>Test passed if :</p> <ol style="list-style-type: none"> Two SCU Diagnostic Science Report telemetry packets are received with the following characteristics: <table border="1" style="margin-left: 40px;"> <thead> <tr> <th>APID</th> <th>Type</th> <th>Subtype</th> <th>SID</th> <th>FrameID</th> <th>Frame length</th> </tr> </thead> <tbody> <tr> <td>0x508</td> <td>21</td> <td>3</td> <td>0x1121</td> <td>0x21</td> <td>0x1E</td> </tr> </tbody> </table> <ol style="list-style-type: none"> The SCU Test Pattern agrees with the reference test pattern. QLA to give go ahead. 	APID	Type	Subtype	SID	FrameID	Frame length	0x508	21	3	0x1121	0x21	0x1E
APID	Type	Subtype	SID	FrameID	Frame length								
0x508	21	3	0x1121	0x21	0x1E								

Test Procedure:

Step#	Action	Comments
1	Write the current values of SCUFRAMECNT located in SCU PARAMETERS display.	
2	Run QLA script FUNC-SCU-08.py on QLA console.	
3	Run FUNC-SCU-08 test procedure from the CCS	
4	When the test is finished Write the current value of SCUFRAMECNT.	
5	Contingency: If test fails repeat steps 1 to 4.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SCU-08	SCUFRAMECNT and SCU test pattern frame parameters	n+62/n+93	62/93	31	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 19 of 105

Start time: 09:59
OBSID:0xb0002bf

CUS Input Default Parameters:
scuframes = 0x1F – Number of SCU frames to generate

Comments: TM5N 3 -> 5

QLA has written file FUNC-SCU-08_B00002BF_8A07.txt:

SCU Test Pattern @ Tue Oct 23 11:00:45 BST 2007
..compared with data from SCU Test Pattern @ Wed Mar 14 14:07:43 GMT 2007, OBSID=0x300125B3

Name	New Value[0]	New Value[20]	Comp Value[0]	Comp Value[20]
SCUTSTOBSID	0xB00002BF	0x0	0x300125B3	0x0
SCUTSTBBID	0x8A070001	0x0	0x8A070001	--> OK 0x0 --> OK
SCUTSTBLKLEN	30.0	30.0	30.0	--> OK 30.0 --> OK
SCUTSTFRAMEID	33.0	33.0	33.0	--> OK 33.0 --> OK
SCUTST001	43690.0	31181.0	43690.0	--> OK 31181.0 --> OK
SCUTST002	21844.0	62363.0	21844.0	--> OK 62363.0 --> OK
SCUTST003	43688.0	59190.0	43688.0	--> OK 59190.0 --> OK
SCUTST004	21840.0	52844.0	21840.0	--> OK 52844.0 --> OK
SCUTST005	43680.0	40153.0	43680.0	--> OK 40153.0 --> OK
SCUTST006	21825.0	14771.0	21825.0	--> OK 14771.0 --> OK
SCUTST007	43650.0	29543.0	43650.0	--> OK 29543.0 --> OK
SCUTST008	21765.0	59086.0	21765.0	--> OK 59086.0 --> OK
SCUTST009	43530.0	52637.0	43530.0	--> OK 52637.0 --> OK
SCUTST010	21524.0	39739.0	21524.0	--> OK 39739.0 --> OK
SCUTST011	43048.0	13943.0	43048.0	--> OK 13943.0 --> OK
SCUTST012	20560.0	27887.0	20560.0	--> OK 27887.0 --> OK
SCUTST013	41120.0	55774.0	41120.0	--> OK 55774.0 --> OK
SCUTST014	16705.0	46012.0	16705.0	--> OK 46012.0 --> OK
SCUTST015	33411.0	26489.0	33411.0	--> OK 26489.0 --> OK
SCUTST016	1287.0	52978.0	1287.0	--> OK 52978.0 --> OK
SCUTST017	2574.0	40420.0	2574.0	--> OK 40420.0 --> OK
SCUTST018	5149.0	15304.0	5149.0	--> OK 15304.0 --> OK
SCUTST019	10298.0	30608.0	10298.0	--> OK 30608.0 --> OK
SCUTST020	20597.0	61216.0	20597.0	--> OK 61216.0 --> OK
SCUTST021	41194.0	56896.0	41194.0	--> OK 56896.0 --> OK
SCUTST022	16852.0	48257.0	16852.0	--> OK 48257.0 --> OK
SCUTST023	33705.0	30978.0	33705.0	--> OK 30978.0 --> OK
SCUTST024	1874.0	61956.0	1874.0	--> OK 61956.0 --> OK
SCUTSTADCFLGS	0.0	0.0	0.0	--> OK 0.0 --> OK
SCUTSTFRAMETIME	4063027.0	4141139.0	4284236.0	4362348.0
SCUTSTCHECKWORD	40139.0	47888.0	15560.0	6994.0



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 20 of 105

Step#	Action	Comments
0	Open MCU_PARAMETERS display on SCOS Alpha Numeric Displays.	

4.9 FUNC-MCU-01: MCU Boot Check

Test Id:	FUNC-MCU-01: MCU Boot Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON
Success Criteria:	Test passed if: <ol style="list-style-type: none"> 1. MCU boots. 2. MCU voltages show expected values. 3. MAC, SMEC and BSM board temperatures shows ambient temperature.

Test Procedure:

Step#	Action	Comments
1	Run FUNC-MCU-01 test procedure from the CCS	
2	When procedure is finished Write the values of the MCU voltages.	
3	Contingency: If test fails repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-MCU-01	MCUP5V MCUP15V MCUP14V MCUM14V MCUM15V MCUMACTEMP MCUSMECTEMP MCUBSMTEMP	N/A / ~ 5V N/A / ~15V N/A / ~ 14V N/A / ~ -14V N/A / ~ -15V N/A / ~ 300K N/A / ~ 300K N/A / ~ 300K	- / 5.01V - / 15.54V - / 14.15V - / -14.47 V - / -15.63 V - / 290.56K - / 295.70K - / 295.29 K	N/A	Success



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 21 of 105

**Start time: 10:01
OBSID:0xb00002C0**

CUS Input Default Parameters: None

**Comments:
MCUBITSTAT went from 0 to 1 as expected**

Test Successful



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	22 of 105

4.10 FUNC-MCU-02: MCU Nominal Frame Generation Check

Test Id:	FUNC-MCU-02: MCU Nominal Frame Generation Check																																			
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON																																			
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON																																			
Success Criteria:	<p>Test passed if :</p> <ol style="list-style-type: none"> MCU produces each type of the frames requested and with the following characteristics. <table border="1"> <thead> <tr> <th>Frame</th> <th>APID</th> <th>Type</th> <th>Subtype</th> <th>SID</th> <th>FrameID</th> <th>Frame length</th> </tr> </thead> <tbody> <tr> <td>Eng.</td> <td>0x508</td> <td>21</td> <td>3</td> <td>0x814</td> <td>0x14</td> <td>0x15</td> </tr> <tr> <td>BSM</td> <td>0x508</td> <td>21</td> <td>1</td> <td>0x612</td> <td>0x12</td> <td>0xD</td> </tr> <tr> <td>SMEC</td> <td>0x508</td> <td>21</td> <td>1</td> <td>0x410</td> <td>0x10</td> <td>0xC</td> </tr> <tr> <td>BSM +SMEC</td> <td></td> <td></td> <td></td> <td></td> <td></td> <td></td> </tr> </tbody> </table> <ol style="list-style-type: none"> No events are generated during the different frames generation. 	Frame	APID	Type	Subtype	SID	FrameID	Frame length	Eng.	0x508	21	3	0x814	0x14	0x15	BSM	0x508	21	1	0x612	0x12	0xD	SMEC	0x508	21	1	0x410	0x10	0xC	BSM +SMEC						
Frame	APID	Type	Subtype	SID	FrameID	Frame length																														
Eng.	0x508	21	3	0x814	0x14	0x15																														
BSM	0x508	21	1	0x612	0x12	0xD																														
SMEC	0x508	21	1	0x410	0x10	0xC																														
BSM +SMEC																																				

Test Procedure:

Step#	Action	Comments
1	Write the current value of MCUFRAMECNT located in MCU_PARAMETERS display	
2	Run QLA script FUNC-MCU-02.py on QLA console.	
3	Run FUNC-MCU-02 test procedure from the CCS	
4	When test is finished Write the current value of MCUFRAMECNT.	
5	Contingency: If test fails repeat steps 1 to 4.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-MCU-02	MCUFRAMECNT	0/ ~ 6600	0 / 6492		Success



Start time: 10:03
OBSID:0xb00002C1

CUS Input Default Parameters:

- f_eng_frames = 64.1Hz – MCU Eng frame generation frequency
f_smec_frames = 250.0Hz – SMEC frame generation frequency
f_bsm_frames = 64.1Hz – BSM frame generation frequency
f_bsmsmec_bsm = 50.0Hz – BSM frame generation frequency for BSM+SMEC
f_bsmsmec_smec = 250.0Hz – SMEC frame generation frequency for BSM+SMEC
ftime = 10 – Time for continuous frame generation for each frame type

QLA generated file QLA-MCU-02_B00002C1.txt :

MCUENG: OBSID = B00002C1, BBTYPE = 0x8901, APID = 0x508, SID = 0x814

Table with 6 columns: Parameter, Initial, Final, Increment, Expect, Packet Chars. Rows include MCUFRAMECNT, TM5N, FrameTime, and statistics on time between reception of 2 consecutive frames.

BSM: OBSID = B00002C1, BBTYPE = 0x8903, APID = 0x508, SID = 0x612

Table with 6 columns: Parameter, Initial, Final, Increment, Expect, Packet Chars. Rows include MCUFRAMECNT, TM5N, FrameTime, and statistics on time between reception of 2 consecutive frames.

SMEC: OBSID = B00002C1, BBTYPE = 0x8902, APID = 0x508, SID = 0x410

Table with 6 columns: Parameter, Initial, Final, Increment, Expect, Packet Chars. Rows include MCUFRAMECNT, TM5N, FrameTime, and statistics on time between reception of 2 consecutive frames.

SMEC+BSM: OBSID = B00002C1, BBTYPE = 0x8904, APID = 0x508, SID = 0x410

Table with 6 columns: Parameter, Initial, Final, Increment, Expect, Packet Chars. Rows include MCUFRAMECNT, TM5N, FrameTime SMEC, FrameTime BSM, and statistics on time between reception of 2 consecutive frames.



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 24 of 105

4.11 FUNC-MCU-03: MCU Nominal Science Contents Check

Test Id:	FUNC-MCU-03: MCU Nominal Contents Check																																			
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON																																			
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON																																			
Success Criteria:	<p>Test passed if :</p> <ol style="list-style-type: none"> MCU produces 99 frames of each type of frames requested with the following characteristics: <table border="1"> <thead> <tr> <th>Frame</th> <th>APID</th> <th>Type</th> <th>Subtype</th> <th>SID</th> <th>FrameID</th> <th>Frame length</th> </tr> </thead> <tbody> <tr> <td>Eng.</td> <td>0x508</td> <td>21</td> <td>3</td> <td>0x814</td> <td>0x14</td> <td>0x15</td> </tr> <tr> <td>BSM</td> <td>0x508</td> <td>21</td> <td>1</td> <td>0x612</td> <td>0x12</td> <td>0xD</td> </tr> <tr> <td>SMEC</td> <td>0x508</td> <td>21</td> <td>1</td> <td>0x410</td> <td>0x10</td> <td>0xC</td> </tr> <tr> <td>BSM +SMEC</td> <td></td> <td></td> <td></td> <td></td> <td></td> <td></td> </tr> </tbody> </table> <ol style="list-style-type: none"> No events are generated during the different frames generation. QLA analysis results are correct. <p>QLA to give go ahead.</p>	Frame	APID	Type	Subtype	SID	FrameID	Frame length	Eng.	0x508	21	3	0x814	0x14	0x15	BSM	0x508	21	1	0x612	0x12	0xD	SMEC	0x508	21	1	0x410	0x10	0xC	BSM +SMEC						
Frame	APID	Type	Subtype	SID	FrameID	Frame length																														
Eng.	0x508	21	3	0x814	0x14	0x15																														
BSM	0x508	21	1	0x612	0x12	0xD																														
SMEC	0x508	21	1	0x410	0x10	0xC																														
BSM +SMEC																																				

Test Procedure:

Step#	Action	Comments
1	Write the current value of MCUFRAMECNT located MCU_PARAMETERS display.	
2	Run QLA script FUNC-MCU-03.py on QLA console.	
3	Run FUNC-MCU-03 test procedure from the CCS	
4	When test is finished Write the current value of MCUFRAMECNT	
5	Contingency: If test fails repeat steps 1 to 4.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-MCU-03	MCUFRAMECNT	n/ n+297 n~6600	6492 / 6789	297	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 25 of 105

Start time: 10:07
OBSID:0xb00002c2

CUS Input Default Parameters:

- n_eng_frames = 100 – Number of MCU Eng frames
- f_eng_frames = 64.1Hz – MCU Eng frame generation frequency
- n_smec_frames = 100 – Number of SMEC frames
- f_smec_frames = 250.0Hz – SMEC frame generation frequency
- n_bsm_frames = 100 – Number of BSM frames
- f_bsm_frames = 64.1Hz – BSM frame generation frequency
- ftime = 10 – Time for continuous frame generation for each frame type (Parameter NA)

Produced 99 frames instead of 100 as expected for each type of MCU frame

QLA produced three files: QLA-MCU-03_B00002C2_8901.txt (SMEC), QLA-MCU-03_B00002C2_8902.txt (MCU Eng) and QLA-MCU-03_B00002C2_8903.txt (BSM).

QLA-MCU-03_B00002C2_8901.txt (SMEC)

Housekeeping Tue Oct 23 10:09:03 UTC 2007
Science Tue Oct 23 10:09:03 UTC 2007

Name	HK before	Science	HK after	Equal (within 10%)?
SMECENC SIG1	12405.0	12406.0	12404.0	True
SMECENC SIG2	20069.0	20070.0	20069.0	True
SMECLVDTDCSIG	32760.0	32758.0	32759.0	True
SMECLVDTAC SIG	27339.0	27338.0	27336.0	True
SMECMOTORCURRE	32778.0	32776.0	32776.0	True
SMECMOTORVOLT	34517.0	34514.0	34521.0	True
CHOPSENS SIG	32766.0	32762.0	32763.0	True
CHOPMOTORCURRE	32777.0	32776.0	32776.0	True
CHOPMOTORVOLT	33636.0	33626.0	33632.0	True
JIGGSENS SIG	32754.0	32755.0	32756.0	True
JIGGMOTORCURRE	32776.0	32772.0	32774.0	True
JIGGMOTORVOLT	33360.0	33360.0	33360.0	True

QLA-MCU-03_B00002C2_8902.txt (MCU Eng)

Housekeeping Tue Oct 23 10:09:20 UTC 2007
Science Tue Oct 23 10:09:20 UTC 2007

Name	HK before	Science	HK after	Equal (within 10%)?
SMECENC POSN	0.0	0.0	0.0	True
SMECENC FINE POSN	0.0	0.0	0.0	True
SMECLVDTDCSIG	32758.0	32760.0	32760.0	True
SMECMOTORBEMF	1748.0	1752.0	1749.0	True

QLA-MCU-03_B00002C2_8903.txt (BSM)

Housekeeping Tue Oct 23 10:09:36 UTC 2007
Science Tue Oct 23 10:09:36 UTC 2007

Name	HK before	Science	HK after	Equal (within 10%)?
CHOPSENS SIG	32763.0	32762.0	32764.0	True
CHOPDACVAL	32768.0	32768.0	32768.0	True
CHOPMOTORVOLT	33637.0	33637.0	33636.0	True
JIGGSENS SIG	32753.0	32756.0	32757.0	True
JIGGDACVAL	32768.0	32768.0	32768.0	True
JIGGMOTORVOLT	33360.0	33360.0	33361.0	True

No discrepancies between HK and science parameter values.



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	26 of 105

4.12 FUNC-MCU-04: MCU Test Pattern Check

Test Id:	FUNC-MCU-04: MCU Test Pattern Check														
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON														
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON														
Success Criteria:	<p>Test passed if:</p> <ol style="list-style-type: none"> MCU produces 100 frames of Test Pattern with the following characteristics: <table border="1"> <thead> <tr> <th>Frame</th> <th>APID</th> <th>Type</th> <th>Subtype</th> <th>SID</th> <th>FrameID</th> <th>Frame length</th> </tr> </thead> <tbody> <tr> <td>Test</td> <td>0x508</td> <td>21</td> <td>3</td> <td>0x915</td> <td>0x15</td> <td>0x15</td> </tr> </tbody> </table> <ol style="list-style-type: none"> MCU Test pattern produced is the same as the previous time this test was run. <p>QLA to give go ahead.</p>	Frame	APID	Type	Subtype	SID	FrameID	Frame length	Test	0x508	21	3	0x915	0x15	0x15
Frame	APID	Type	Subtype	SID	FrameID	Frame length									
Test	0x508	21	3	0x915	0x15	0x15									

Test Procedure:

Step#	Action	Comments
1	Write the current value of MCUFRAMECNT located in MCU_PARAMETERS display.	
2	Run QLA script FUNC-MCU-04.py on QLA console.	
3	Run FUNC-MCU-04 test procedure from the CCS	
4	When test is finished Write the current value of MCUFRAMECNT	
5	Contingency: If test fails repeat steps 1 to 4.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-MCU-04	MCUFRAMECNT	m/ m+99 m~6600	6789 / 6888	99	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 27 of 105

Start time: 10:10
OBSID:0xb00002c3

CUS Input Default Parameters:

n_test_frames = 100 – Number of MCU Test Pattern frames
f_test_frames = 64.1Hz – MCU Test Pattern frame generation frequency

Comments:

Produced 99 frames instead of 100 as expected.

QLA generated file QLA-MCU-04_ B00002C3_8905.txt:

MCU Test Pattern @ Tue Oct 23 10:12:06 UTC 2007
..compared with data from MCU Test Pattern @ Wed Mar 14 14:31:00 GMT 2007, OBSID=0x300125B9

Name	New Value[0]	New Value[20]	Comp Value[0]	Comp Value[20]
MCUTSTOBSID	0xB00002C3	0x0	0x300125B9	0x0
MCUTSTBBID	0x89050001	0x0	0x89050001	0x0
MCUTSTBLKLEN	21.0	21.0	21.0	21.0
MCUTSTFRAMEID	21.0	21.0	21.0	21.0
MCUTSTACQTIME	3755011.0	3857784.0	3994451.0	4097224.0
MCUTST001	21845.0	21845.0	21845.0	21845.0
MCUTST002	43690.0	43690.0	43690.0	43690.0
MCUTST003	21844.0	21844.0	21844.0	21844.0
MCUTST004	43688.0	43688.0	43688.0	43688.0
MCUTST005	21840.0	21840.0	21840.0	21840.0
MCUTST006	43680.0	43680.0	43680.0	43680.0
MCUTST007	21825.0	21825.0	21825.0	21825.0
MCUTST008	43650.0	43650.0	43650.0	43650.0
MCUTST009	21765.0	21765.0	21765.0	21765.0
MCUTST010	43530.0	43530.0	43530.0	43530.0
MCUTST011	21524.0	21524.0	21524.0	21524.0
MCUTST012	43048.0	43048.0	43048.0	43048.0
MCUTST013	20560.0	20560.0	20560.0	20560.0
MCUTST014	41120.0	41120.0	41120.0	41120.0
MCUTSTTIME	3755486.0	3858258.0	3994925.0	4097699.0
MCUTSTCHECKWORD	61998.0	61913.0	62861.0	61848.0

Comparison successful



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	28 of 105

Step#	Action	Comments
0	Open CHOP & JIGGLE PARAMETERS displays on SCOS Alpha Numeric Displays.	

4.13 FUNC-BSM-01: BSM Chop/Jiggle Sensor Check

Test Id:	FUNC-BSM-01: BSM Chop/Jiggle Sensor Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Success Criteria:	Test passed if: <ol style="list-style-type: none"> 1. CHOPSENSPWR HK parameter goes from 0 to 1 2. CHOPDACVAL HK parameter stays at or goes to 0x8000 3. CHOPSENSIG HK parameter shows variation from off to on 4. JIGGSENSPWR HK parameter goes from 0 to 1 5. JIGGDACVAL parameter stays at or goes to 0x8000 6. JIGGSENSSIG HK parameter shows variation from off to on

Test Procedure

Step#	Action	Comments
1	On QLA bring up a time series display of the following HK parameters: CHOPSENSPWR CHOPDACVAL CHOPSENSIG JIGGSENSPWR JIGGDACVAL JIGGSENSSIG	
2	Run FUNC-BSM-01 test procedure from the CCS	
3	When the test is finished record all the Key parameters noted below	
	Contingency: If test fails repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-BSM-01	CHOPSENSPWR CHOPLOOPMODE CHOPDACVAL CHOPFFGAIN CHOPSENSSIG JIGGSENSPWR JIGGLOOPMODE JIGGDACVAL JIGGFFGAIN JIGGSENSSIG	0/1 3/3 0x8000/0x8000 0xBEB/0x700 ~0x8000 0/1 3/3 0x8000/0x8000 0xBEB/0xF6E ~0x8000/?	0/1 3/3 0x8000/0x8000 0xBEB/0x770 ~0x7FFE/~0x8EB9 0/1 3/3 0x8000/0x8000 0xBEB/0xF6E 0x7FF2/~ 0x8F3A	N/A	Success



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	29 of 105

Start time: 10:15

OBSID:0xb00002c4

CUS Input Default Parameters: None

Comments:

The BSM was switched ON correctly. The Chop and Jiggle FF gains are consistent with the latest BSMNominalSettings.txt table in the CUS.



SPIRE Document
IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	30 of 105

4.14 FUNC-BSM-02C: BSM Chop Sensor Polarity Check

Test Id:	FUNC-BSM-02C: BSM Chop Sensor Polarity Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Success Criteria:	Test passed if the chop sensor signal evolves in the same way as the positions set.(i.e if (pos1 > pos2 → sig1 > sig2)

Test Procedure:

Step#	Action	Comments
1	On QLA open up a time series display of HK parameter CHOPDACVAL and CHOPSENSSIG	
2	Run FUNC-BSM-02C test procedure from the CCS	
3	Contingency: If test fails repeat steps 1.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-BSM-02C	CHOPDACVAL CHOPSENSSIG		See below	N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King


Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 31 of 105

Start time: 10:22
OBSID:0xb00002c5

CUS Input Default Parameters: None

Comments:
The BSM moved along the chop axis in the same direction as expected.

QLA plots:

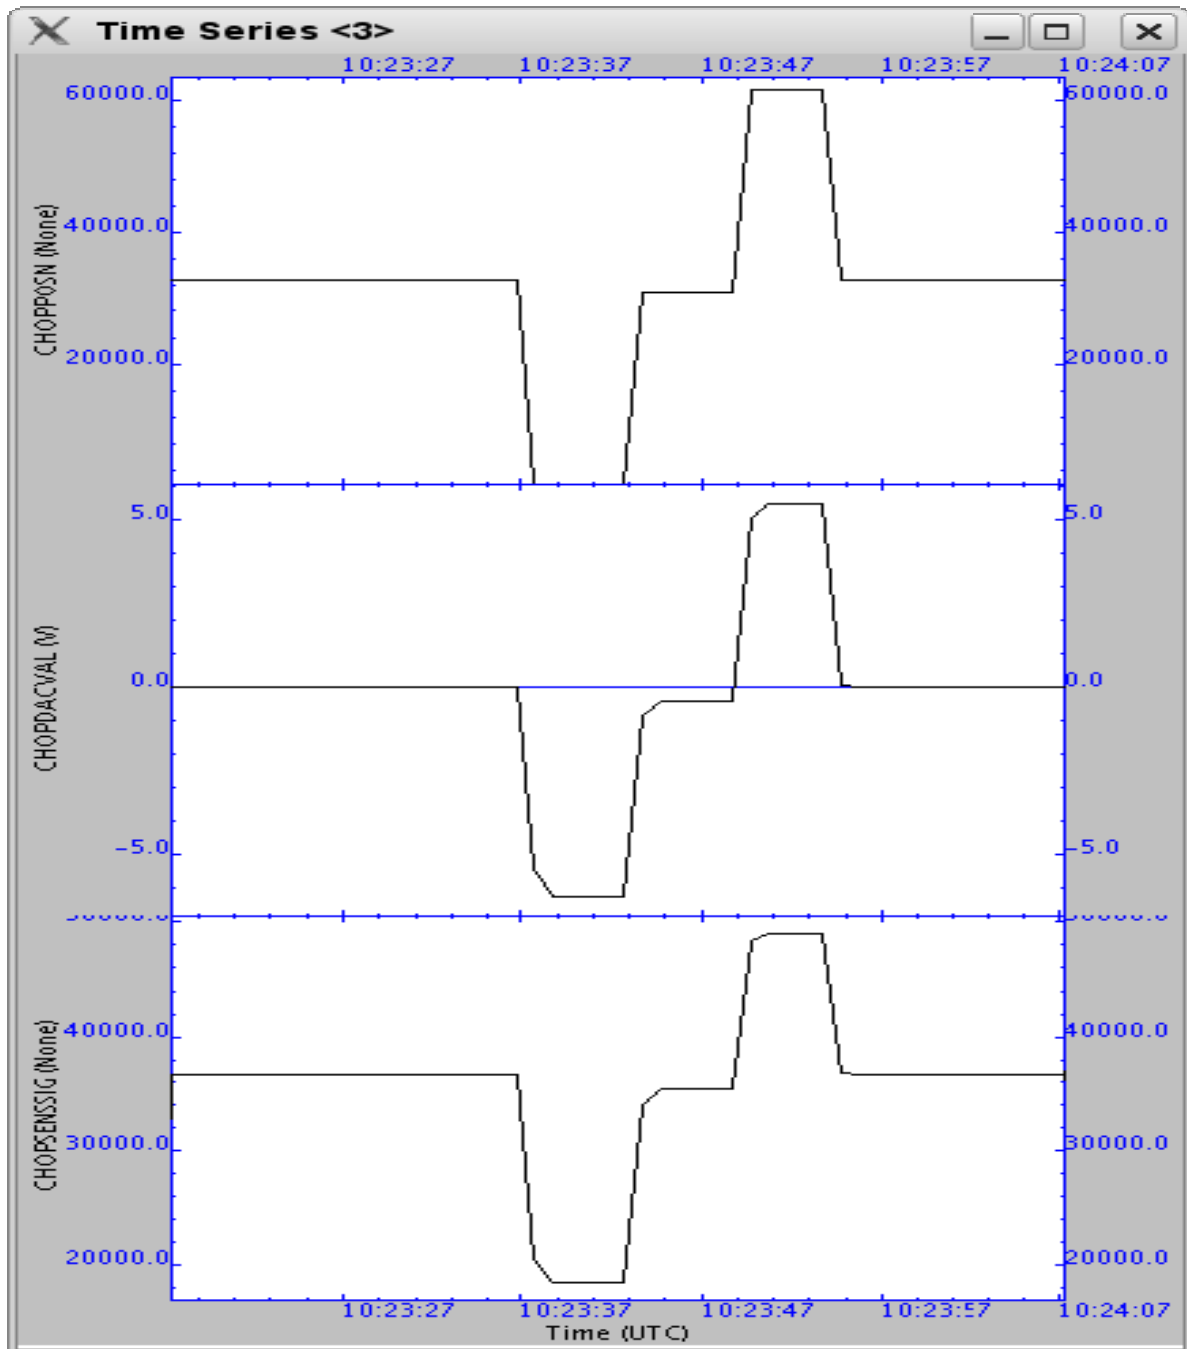



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 32 of 105

4.15 FUNC-BSM-02J: BSM Jiggle Sensor Polarity Check

Test Id:	FUNC-BSM-02J: BSM Jiggle Sensor Polarity Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Success Criteria:	Test passed if the jiggle sensor signal evolves in the same way as the positions set.(i.e if (pos1 > pos2 → sig1 > sig2)

Test Procedure:

Step#	Action	Comments
1	On QLA open up a time series display of HK parameter JIGGDACVAL and JIGGSENSSIG	
2	Run FUNC-BSM-02J test procedure from the CCS	
3	Contingency: If test fails repeat steps 1.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-BSM-02J	JIGGDACVAL JIGGSENSSIG		See below	N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King


Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 33 of 105

Start time: 10:29
OBSID:0xb00002c6

CUS Input Default Parameters: None

Comments:
The BSM moved along the jiggle axis in the same direction as expected.

QLA plots:

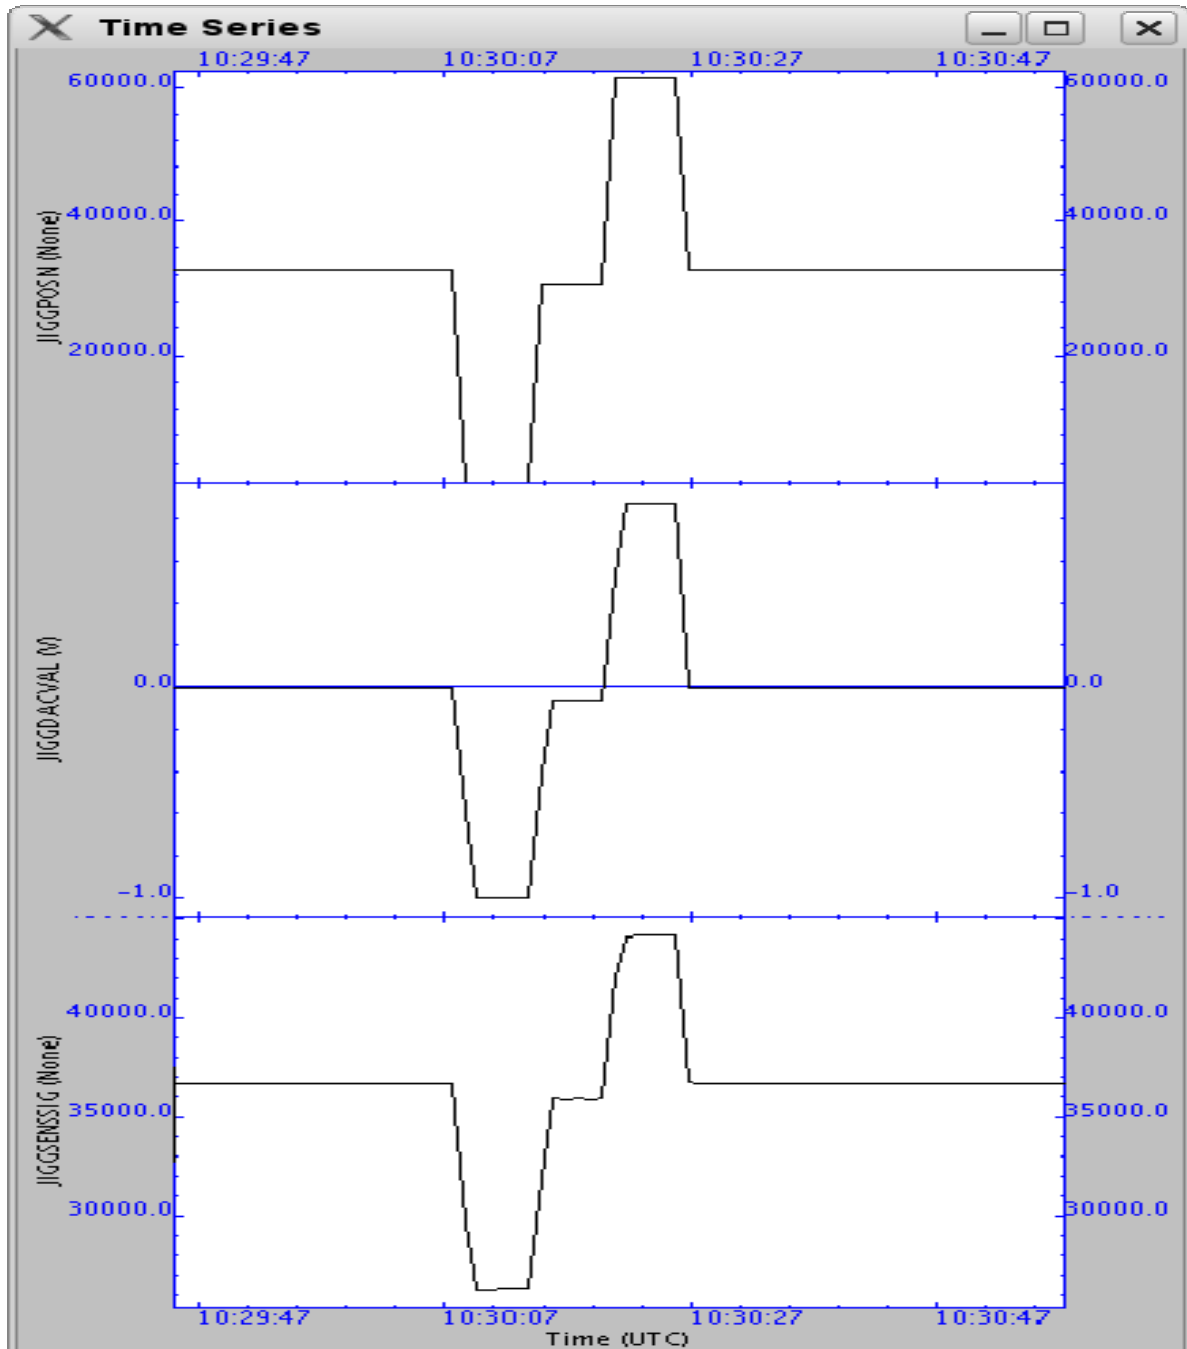



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	34 of 105

4.16 FUNC-BSM-03: BSM Open Loop Dynamics Check

Test Id:	FUNC-BSM-03: BSM Open Loop Dynamics Test
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Success Criteria:	Test passed if the chop sensor signal evolves in the same way as the positions set.(i.e if (pos1 > pos2 → sig1 > sig2) for each jiggle position. Note: During warm tests the voltages on both chop and jiggle motors are likely to be saturated (CHOP/JIGGMOTORVOLT RAW values of ~ 0xFFFF) due to the high resistance of the motor coil at ambient temperature.

Test Procedure

Step#	Action	Comments
1	On QLA open up a time series display of HK parameters: CHOPPOSN CHOPDACVAL CHOPMOTORCURRE CHOPSENSSIG CHOPMOTORVOLT JIGGPOSN JIGGDACVAL JIGGMOTORCURRE JIGGSENSSIG JIGGMOTORVOLT	
2	Run FUNC-BSM-03 test procedure from the CCS	
3	Contingency: If test fails repeat step 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-BSM-03				N/A	Success



Start time: 10:34

OBSID:0xb00002c7

CUS Input Default Parameters:


```
string frametype = "BSM"; // Specifies MCU frame type [  
double framerate = 64.0; // Specifies the frame rate  
int j_start = 0x4000; // RAW jiggle target start position  
int j_end = 0xc000; // RAW jiggle target end position  
int j_step = 0x4000; // RAW jiggle target step in position  
int j_delay = 2; // Time at each jiggle target position in seconds  
int c_start = 0x3000; // RAW chop target start position  
int c_end = 0xf000; // RAW chop target end position  
int c_step = 0x1000; // RAW chop target step in position  
int c_delay = 5; // Time at each chop target position in seconds
```

Comments:

MCUFRAMECNT: 6888 -> 22676


Jiggle position as given by senssig shows going to position then coming back as the chop position is stepped. This is due to the coupling between the axes.

QLA plots for Chop Axis:

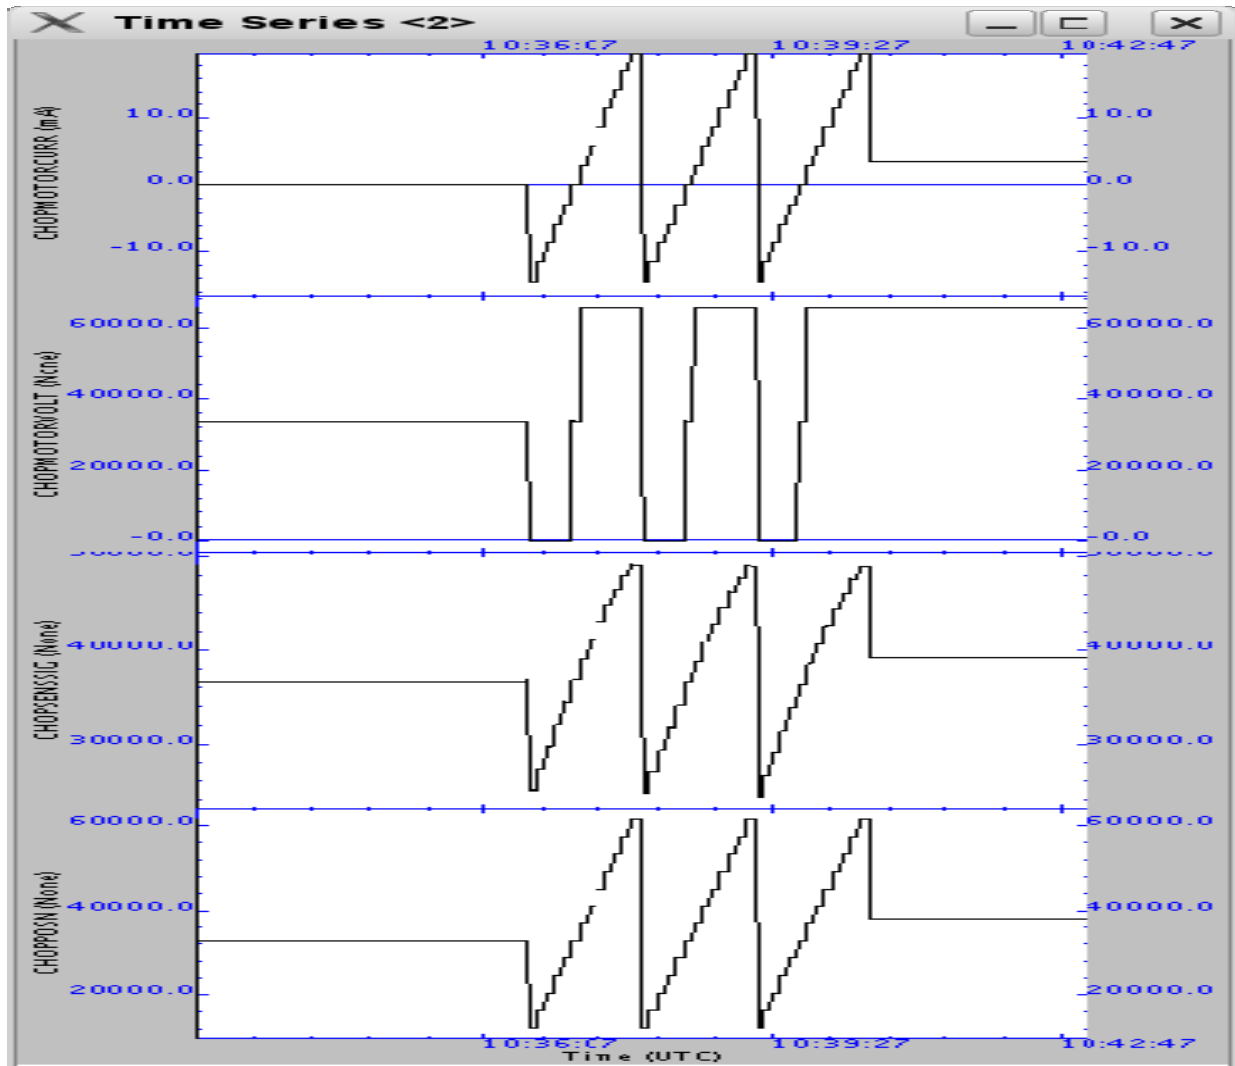



QLA plots for Jiggle Axis:

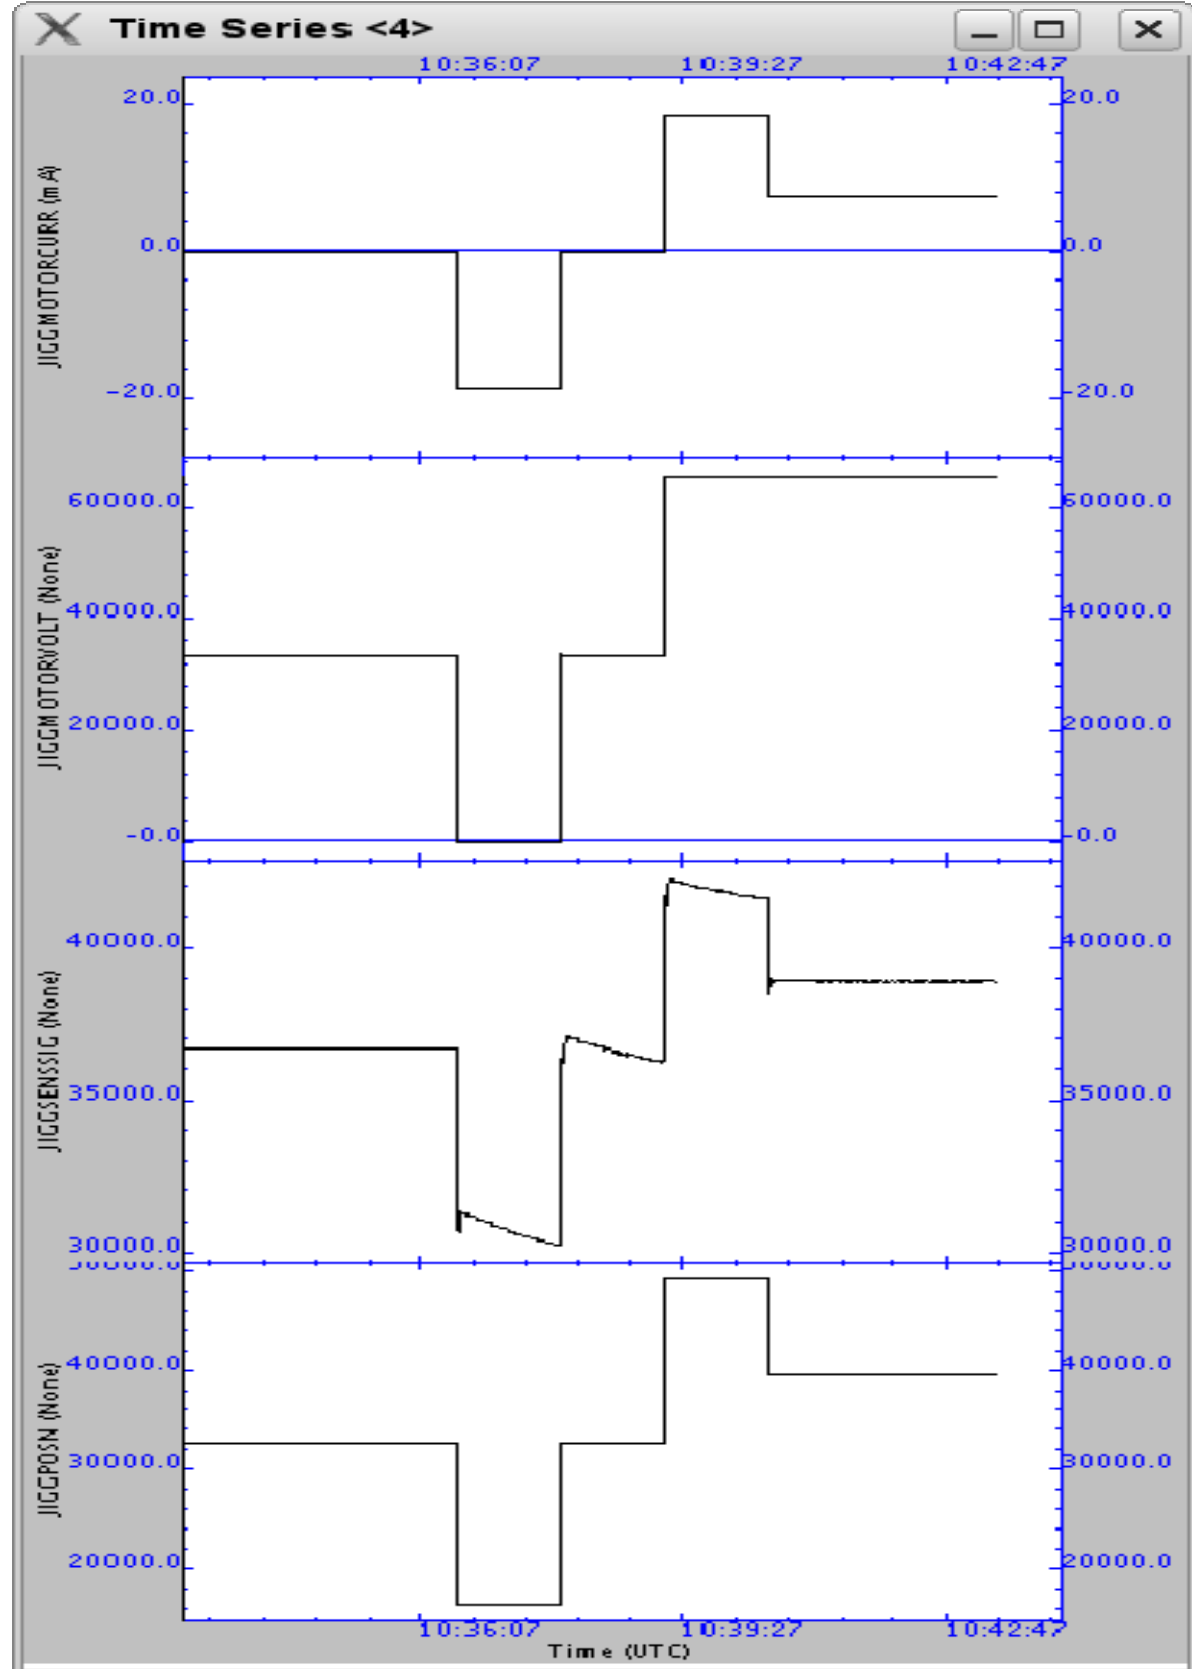



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	37 of 105

4.17 FUNC-BSM-05A: BSM Open Loop Chop Test

Test Id:	FUNC-BSM-05A: Open Loop Chop Test
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Success Criteria:	Note: The purpose of this test is to check the correctness of the BSM open loop chop test.

Test Procedure

Step#	Action	Comments
1	On QLA open up a time series display of HK parameters: BSMCHOPSENSSIG BSMCHOPMOTORCURR BSMCHOPMOTORVOLT BSMJIGGSENSSIG BSMJIGGMOTORCURR BSMJIGGMOTORVOLT	
2	Run FUNC-BSM-05A test procedure from the CCS	
3	Contingency: None contemplated.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-BSM-05A				N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	38 of 105

Start time: 10:45

OBSID:0xb00002c8

CUS Input Default Parameters:

```
string frametype = "BSM"; // Specifies MCU frame type
double framerate = 125.0; // Specifies the frame rate
int on_source_chop = 0xa000; // On source chop position
int on_source_jiggle = 0x8000; // On source jiggle position
int off_source_chop = 0x8000; // Off source chop position
int off_source_jiggle = 0x8000; // Off source jiggle position
int ncycles = 50; //Number of chop cycles
int chop_period = 500000; //period of chop cycles in microsec
int dcumode = 0; //Data type
int dcusample = 4; //Number of DCU samples per chop position
int dcudelay = 34959; //Dealy to start sampling the DCU
int bsmsample = 31; //Number of BSM samples per position
```


Comments: Plots from QLA below



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 39 of 105

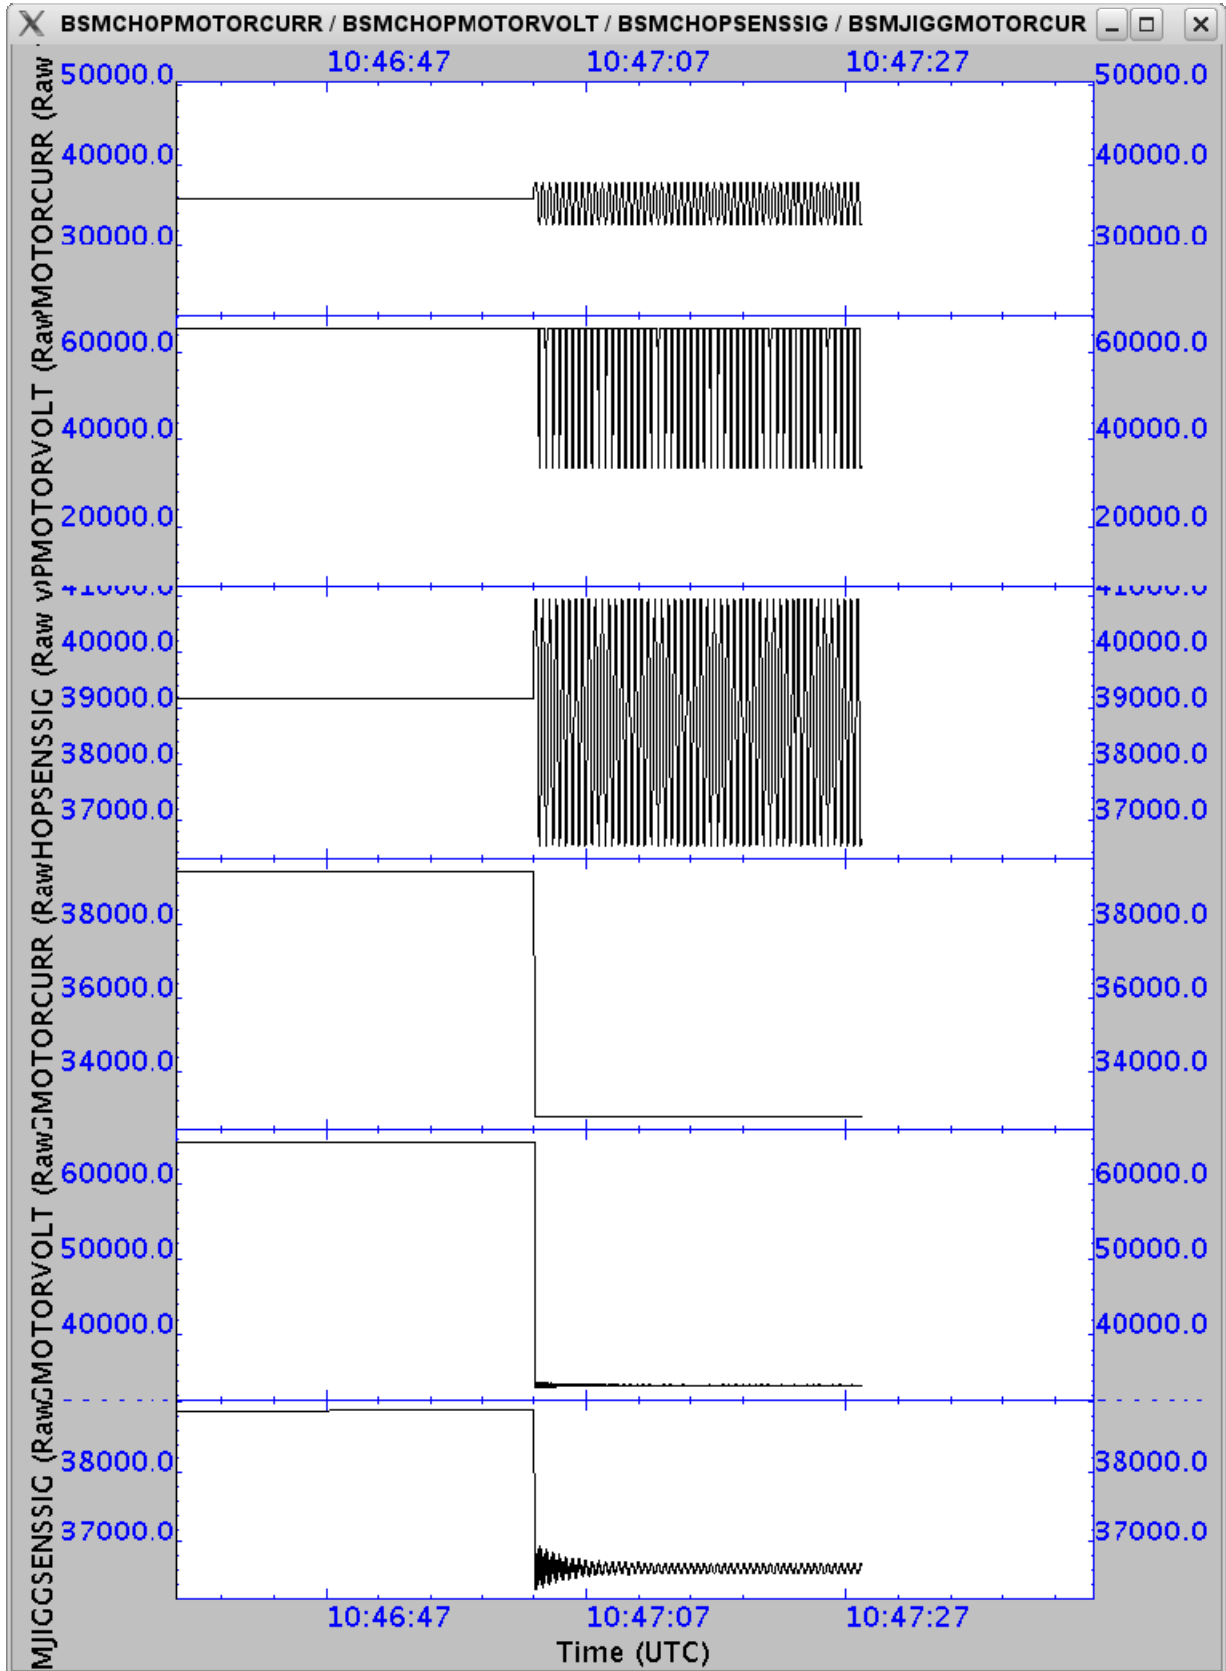



4.18 FUNC-BSM-05B: BSM Closed Loop Chop Test

Test Id:	FUNC-BSM-05B: BSM Closed Loop Chop Test
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Success Criteria:	<p>Note: The purpose of this test is to check the correctness of the BSM close loop initialisation procedure and the default PID parameters</p> <p>If the dynamical behaviour of the BSM during chopping with these PID parameters is close or within requirements this indicates that the PID parameters used can be applied to cold testing with certain adjustment. If NOT these indicates that the PID parameters need further tuning BUT NOT TO BE DONE DURING THESE TEST.</p> <p>In any case the success/fail criteria are NOT applicable for this test.</p>

Test Procedure

Step#	Action	Comments
1	On QLA open up a time series display of HK parameters: BSMCHOPSENSSIG BSMCHOPMOTORCURRE BSMCHOPMOTORVOLT BSMJIGGSENSSIG BSMJIGGMOTORCURRE BSMJIGGMOTORVOLT	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-BSM-05B	CHOPLOOPMODE JIGGLOOPMODE	3/1 3/1		N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 41 of 105

10:52 BSM_INIT
OBSID:0xb00002c9
CHOPLOOPMODE 3 to 1
JIGGLOOPMODE 3 to 1

Comments:

10:54 BSM-05B
OBSID:0xb00002ca

CUS Input Default Parameters:

```
string frametype = "BSM"; // Specifies MCU frame type
double framerate = 125.0; // Specifies the frame rate
int on_source_chop = 0xb600; // On source chop position
int on_source_jiggle = 0x9a60; // On source jiggle position
int off_source_chop = 0x6a28; // Off source chop position
int off_source_jiggle = 0x9a60; // Off source jiggle position
int ncycles = 50; //Number of chop cycles
int chop_period = 500000; //period of chop cycles in microsec
int dcumode = 0; //Data type
int dcusample = 4; //Number of DCU samples per chop position
int dcudelay = 34959; //Dealy to start sampling the DCU
int bsmsample = 31; //Number of BSM samples per position
```

Plots from QLA for 0xb00002ca:



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	42 of 105

4.19 FUNC-BSM-06: BSM Operational Mode Check

Test Id:	FUNC-BSM-05B: BSM Operational Mode Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + BSM ON (open loop)
Success Criteria:	Note: The purpose of this test is to check the operational behaviour of the BSM in closed loop.

Test Procedure

Step#	Action	Comments
1	On QLA open up a time series display of HK parameters: BSMCHOPSENSSIG BSMCHOPMOTORCURRE BSMCHOPMOTORVOLT BSMJIGSENSSIG BSMJIGMOTORCURRE BSMJIGMOTORVOLT	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-BSM-06				N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 43 of 105

Start time: 10:57

OBSID:0xb00002cb

CUS Input Default Parameters:

```
string frametype = "BSM"; // Specifies MCU frame type]
double framerate = 125.0; // Specifies the frame rate
int on_source_chop = 0x5279; // On source chop position
int on_source_jiggle = 0x8d00; // On source jiggle position
int off_source_chop = 0xad87; // Off source chop position
int off_source_jiggle = 0x8d00; // Off source jiggle position
int ncycles = 50; //Number of chop cycles
int chop_period = 500000; //period of chop cycles in microsec
int dcumode = 0; //Data type
int dcusample = 4; //Number of DCU samples per chop position
int dcudelay = 34959; //Dealy to start sampling the DCU
int bsmsample = 65535; //Number of BSM samples per position
```

Comments: **Transparent packets seen on the CCS.**


Output from QLA script for BSM-06 below.



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 44 of 105

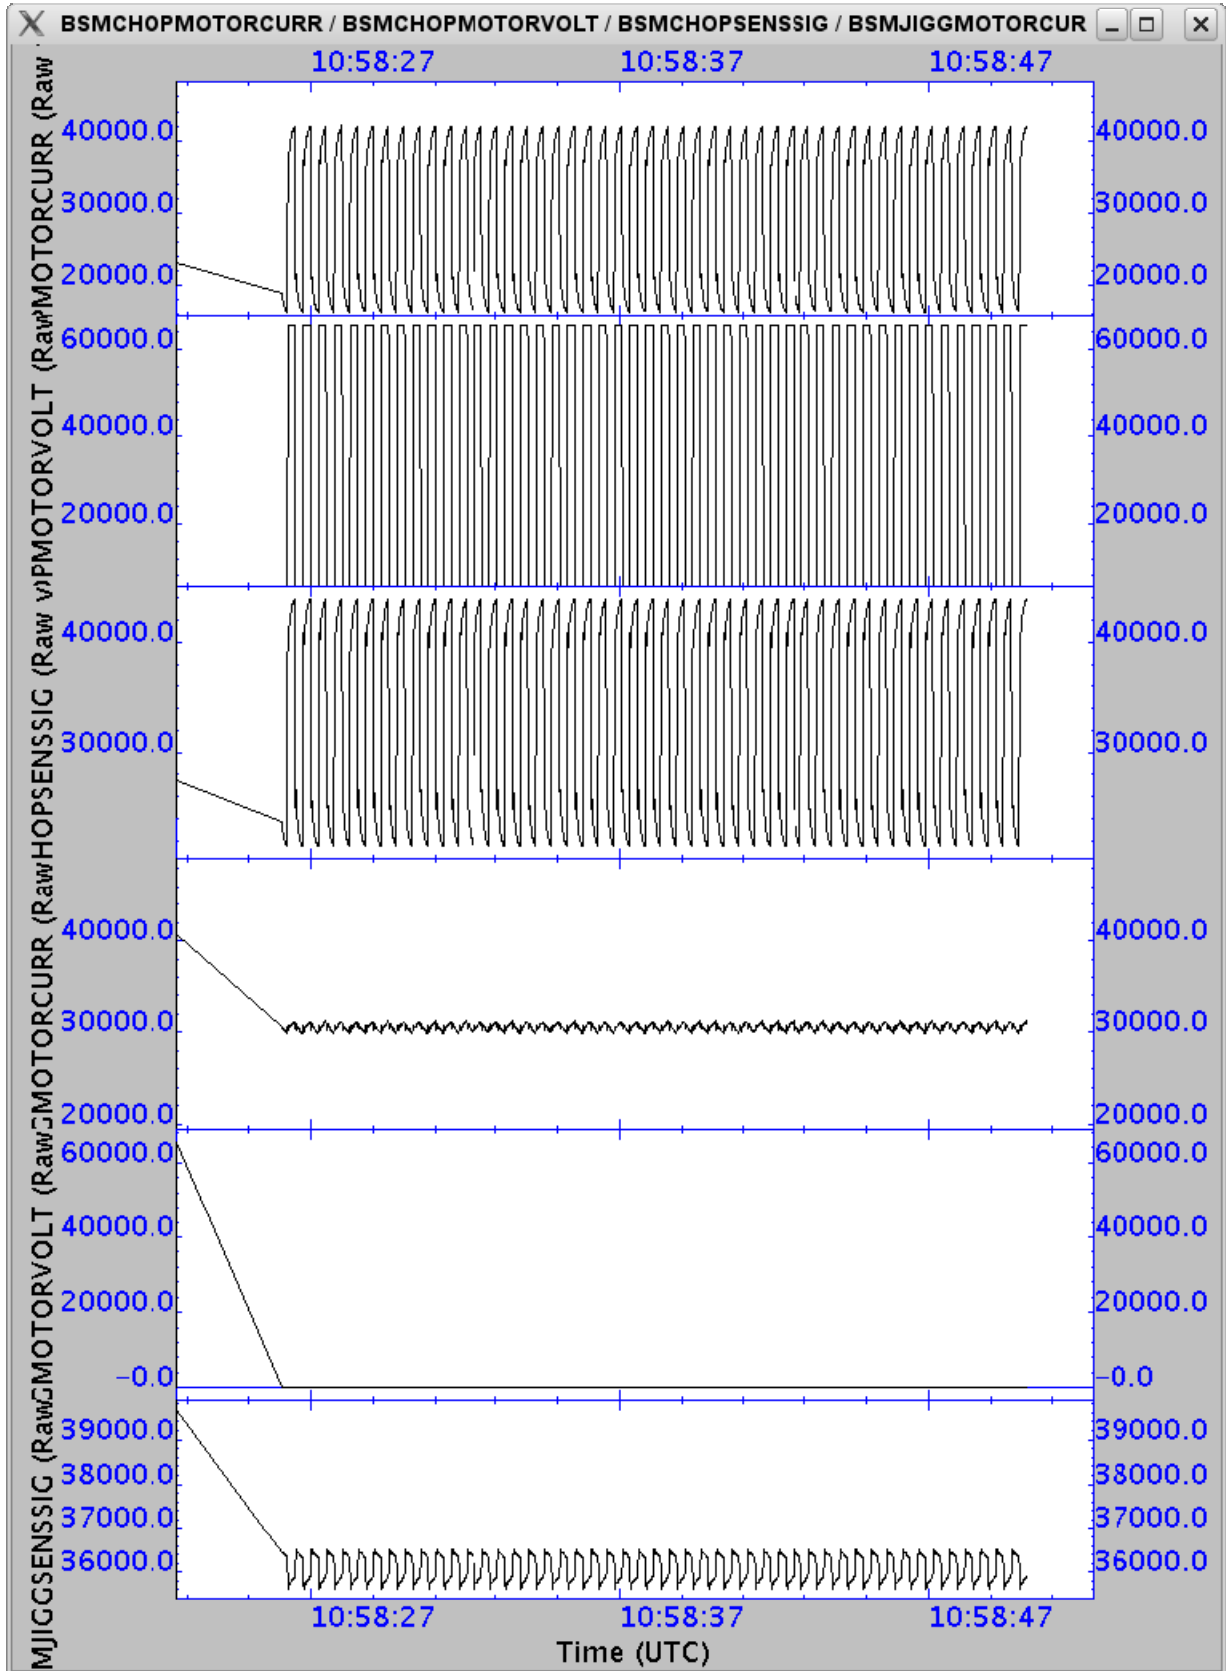



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 45 of 105

BSM_OFF:

Start time: 10:01

OBSID: 0xb00002cc

CHOP/JIGGLOPPMODE 1 to 3

CHOP/JIGGSENPWR: 1 to 0

Step#	Action	Comments
0	Open DCU PARAMETERS SCOS Alpha Numeric Display	

4.20 FUNC-DCU-01: DCU Nominal Science Packet Generation Check

Test Id:	FUNC-DCU-01: DCU Nominal Science Packet Generation Check																																																														
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON																																																														
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON																																																														
Success Criteria:	Test passed if: <ol style="list-style-type: none"> DCU produces each type of DCU nominal science frame with the following characteristics. <table border="1"> <thead> <tr> <th>APID</th> <th>Type</th> <th>S.type</th> <th>SID</th> <th>Frame ID</th> <th>Frame type</th> <th>Nb. Of frames</th> <th>Nb. of pkts.</th> </tr> </thead> <tbody> <tr> <td>0x504</td> <td>21</td> <td>1</td> <td>0x200</td> <td>0</td> <td>PF</td> <td>100</td> <td>100</td> </tr> <tr> <td>0x506</td> <td>21</td> <td>1</td> <td>0x201</td> <td>1</td> <td>SF</td> <td>100</td> <td>17</td> </tr> <tr> <td>0x504</td> <td>21</td> <td>2</td> <td>0x102</td> <td>2</td> <td>PSW</td> <td>100</td> <td>34</td> </tr> <tr> <td>0x504</td> <td>21</td> <td>2</td> <td>0x103</td> <td>3</td> <td>PMW</td> <td>100</td> <td>25</td> </tr> <tr> <td>0x504</td> <td>21</td> <td>2</td> <td>0x104</td> <td>4</td> <td>PLW</td> <td>100</td> <td>12</td> </tr> <tr> <td>0x506</td> <td>21</td> <td>2</td> <td>0x105</td> <td>5</td> <td>SSW</td> <td>100</td> <td>12</td> </tr> </tbody> </table>							APID	Type	S.type	SID	Frame ID	Frame type	Nb. Of frames	Nb. of pkts.	0x504	21	1	0x200	0	PF	100	100	0x506	21	1	0x201	1	SF	100	17	0x504	21	2	0x102	2	PSW	100	34	0x504	21	2	0x103	3	PMW	100	25	0x504	21	2	0x104	4	PLW	100	12	0x506	21	2	0x105	5	SSW	100	12
APID	Type	S.type	SID	Frame ID	Frame type	Nb. Of frames	Nb. of pkts.																																																								
0x504	21	1	0x200	0	PF	100	100																																																								
0x506	21	1	0x201	1	SF	100	17																																																								
0x504	21	2	0x102	2	PSW	100	34																																																								
0x504	21	2	0x103	3	PMW	100	25																																																								
0x504	21	2	0x104	4	PLW	100	12																																																								
0x506	21	2	0x105	5	SSW	100	12																																																								



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	46 of 105

	0x506	21	2	0x106	6	SLW	100	7
<p>2. The frame time difference between consecutive DCU frames of each type corresponds to the sampling rate. Photometer Sampling rate is 15.3Hz → Δt ~ 65.5 ms Spectrometer Sampling rate is 80Hz → Δt = 12.5 ms</p> <p>3. The SPIRE HK parameter DCUFRAMECNT increments by 700.</p> <p>4. No events are generated during the frames generation.</p>								

Test Procedure:

Step#	Action	Comments
1	Write the current value of DCUFRAMECNT located d in DCU PARAMETERS AND	
2	Run FUNC-DCU-01 test procedure from the CCS	
3	Write the current value of DCUFRAMECNT located d in DCU PARAMETERS AND	
4	Contingency: If test fails repeat steps 1 to 3.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-01	DCUFRAMECNT	n/n+700 n depends on the BSM chop operations on FUNC-BSM-06	1200 / 1900	700	Success

Start time: 11:03
OBSID:0xb00002cd

CUS Input Default Parameters:
 double photbiasfreq = 130.0;
 double photosampfreq = 18.0;
 double specbiasfreq = 160.0;
 double specsampfreq = 80.0;
 int frames = 100;

Comments: CCS cannot carry out step 2 of the DCU-01 as they cannot see science packets on their system in the new version

QLA created file QLA-DCU-01_B00002CD.txt:

 PHOTF: OBSID = B00002CD, BBTYP = 0x8800, APID = 0x504, SID = 0x200

Parameter	Initial	Final	Increment	Expect	Incr.	Packet Chars.
DCUFRAMECNT	1200	1300	100	100		Packet type = 0x15



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	47 of 105

TM3N	1199	1299	100	100	subtype = 0x1
FrameTime	53.7600	53.7600			Frame ID = 0x0 Frame Len = 0x126
STATISTICS ON TIME BETWEEN RECEPTION OF 2 CONSECUTIVE FRAMES:					
mean = 53.75938 ms					
sigma = 0.00127 ms					

PHOTSW: OBSID = B00002CD, BBTYPE = 0x8802, APID = 0x504, SID = 0x102					
Parameter	Initial	Final	Increment	Expect	Incre. Packet Chars.
DCUFRAMECNT	1300	1400	100	100	Packet type = 0x15
TM3N	1299	1333	34	34	subtype = 0x2
FrameTime	53.7568	53.7600			Frame ID = 0x2 Frame Len = 0x96
STATISTICS ON TIME BETWEEN RECEPTION OF 2 CONSECUTIVE FRAMES:					
mean = 53.75935 ms					
sigma = 0.00131 ms					

PHOTMW: OBSID = B00002CD, BBTYPE = 0x8803, APID = 0x504, SID = 0x103					
Parameter	Initial	Final	Increment	Expect	Incre. Packet Chars.
DCUFRAMECNT	1400	1500	100	100	Packet type = 0x15
TM3N	1333	1358	25	25	subtype = 0x2
FrameTime	53.7600	53.7568			Frame ID = 0x3 Frame Len = 0x66
STATISTICS ON TIME BETWEEN RECEPTION OF 2 CONSECUTIVE FRAMES:					
mean = 53.75936 ms					
sigma = 0.00127 ms					

PHOTLW: OBSID = B00002CD, BBTYPE = 0x8804, APID = 0x504, SID = 0x104					
Parameter	Initial	Final	Increment	Expect	Incre. Packet Chars.
DCUFRAMECNT	1500	1600	100	100	Packet type = 0x15
TM3N	1358	1370	12	12	subtype = 0x2
FrameTime	53.7568	53.7600			Frame ID = 0x4 Frame Len = 0x36
STATISTICS ON TIME BETWEEN RECEPTION OF 2 CONSECUTIVE FRAMES:					
mean = 53.75935 ms					
sigma = 0.00129 ms					

SPECF: OBSID = B00002CD, BBTYPE = 0x8801, APID = 0x506, SID = 0x201					
Parameter	Initial	Final	Increment	Expect	Incre. Packet Chars.
DCUFRAMECNT	1600	1700	100	100	Packet type = 0x15
TM4N	16383	16	16	17	subtype = 0x1
FrameTime	12.4928	12.4928			Frame ID = 0x1 Frame Len = 0x4E
STATISTICS ON TIME BETWEEN RECEPTION OF 2 CONSECUTIVE FRAMES:					
mean = 12.49263 ms					
sigma = 0.00074 ms					

SPECSSW: OBSID = B00002CD, BBTYPE = 0x8805, APID = 0x506, SID = 0x105					
Parameter	Initial	Final	Increment	Expect	Incre. Packet Chars.
DCUFRAMECNT	1700	1800	100	100	Packet type = 0x15
TM4N	16	28	12	12	subtype = 0x2
FrameTime	12.4928	12.4928			Frame ID = 0x5 Frame Len = 0x36
STATISTICS ON TIME BETWEEN RECEPTION OF 2 CONSECUTIVE FRAMES:					
mean = 12.49265 ms					



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 48 of 105

sigma = 0.00066 ms

SPECLW: OBSID = B00002CD, BBTYPE = 0x8806, APID = 0x506, SID = 0x106

Parameter	Initial	Final	Increment	Expect	Incre.	Packet Chars.
DCUFRAMECNT	1800	1900	100	100		Packet type = 0x15
TM4N	28	35	7	7		subtype = 0x2
FrameTime	12.4928	12.4928				Frame ID = 0x6 Frame Len = 0x1E

STATISTICS ON TIME BETWEEN RECEPTION OF 2 CONSECUTIVE FRAMES:
mean = 12.49264 ms
sigma = 0.00071 ms



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 49 of 105

4.21 FUNC-DCU-02: DCU High Speed Link Check

Test Id:	FUNC-DCU-02: DCU High Speed Link Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON
Success Criteria:	<p>Test passed if DCUFRAMECNT goes from 700 to 1400 and the frametime difference between consecutive frames computed by QLA script is in agreement with the expected differences based on commanded sampling rate:</p> <ol style="list-style-type: none"> 1. Photometer Sampling rate is 15.3Hz → Δt ~ 65.5 ms 2. Spectrometer Sampling rate is 80Hz → Δt = 12.5 ms

Test Procedure:

Step#	Action	Comments
1	Write the current value of DCUFRAMECNT located d in DCU PARAMETERS AND	
2	Run QLA script FUNC-DCU-02.py on QLA console.	
3	Run FUNC-DCU-02 test procedure from the CCS	
4	Write the current value of DCUFRAMECNT located d in DCU PARAMETERS AND	
5	Contingency: If test fails repeat steps 1 to 4.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-02	DCUFRAMECNT	m/m+1400	1900 / 2600	700	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 50 of 105

Start time: 11:08

OBSID: 0xb00002ce

CUS Input Default Parameters:

```
double photbiasfreq = 200.0;  
double photosampfreq = 15.3;  
double specbiasfreq = 160.0;  
double specsampfreq = 80.0;  
int frames = 100;
```

Comments:

QLA script produced 7 files, QLA-DCU-02_B00002CE_880<n>.txt – where n=0 to 6

Contents of QLA created files show sampling times to be consistent with input parameters entered for sampling frequencies of photometer ~15.3Hz ($\Delta t \sim 65.5$ ms) and spectrometer 80Hz $\Delta t \sim 12.5$ ms.



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	51 of 105

4.22 FUNC-DCU-03: DCU Test Pattern Check

Test Id:	FUNC-DCU-03: DCU Test Pattern Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON
Success Criteria:	Test passed if : <ol style="list-style-type: none"> DCU produces 100 frames of Full Photometer Test Pattern and 100 frame of Full Spectrometer Test Pattern test. QLA analysis shows that phot/spec test patterns are the same as the reference phot/spec test patterns.

Test Procedure:

Step#	Action	Comments
1	Write the current value of DCUFRAMECNT located d in DCU PARAMETERS AND	
2	Run QLA script FUNC-DCU-03.py on QLA console.	
3	Run FUNC-DCU-03 test procedure from the CCS	
4	Write the current value of DCUFRAMECNT located d in DCU PARAMETERS AND	
5	Contingency: If test fails repeat steps 1 to 4.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-03	DCUFRAMECNT	j/j+200	2600 / 2800	200	Success



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 52 of 105

Start time: 11:13

OBSID: 0xb00002cf

CUS Input Default Parameters:

double photbiasfreq = 200.0;
double photosampfreq = 15.3;
double specbiasfreq = 160.0;
double specsampfreq = 80.0;
int phase = 0;
int frames = 100;

Comments:

Files produced by QLA:

QLA-DCU-03_B00002CF_8807.txt – DCU Photometer Test Pattern
QLA-DCU-03_B00002CF_8808.txt – DCU Spectrometer Test Pattern

Test pattern file shows agreement with reference DCU test pattern files– see Annexe 1



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	53 of 105

4.23 FUNC-DCU-04-PHOT: Photometer LIAs Check

Test Id:	FUNC-DCU-04P: Photometer LIAs Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Photometer LIAs ON
Success Criteria:	Test passed if : <ol style="list-style-type: none"> SCUDCDCSTAT parameter goes from 4 to 5. Photometer LIA card voltages are showing correct readings of +5V,+9V,-9V. Photometer LIA temperatures show an increase indicating that they are ON.

Test Procedure:

Step#	Action	Comments
1	On QLA bring up a time series display of the HK parameters: PLIAP5V PLIAP9V PLIAM9V LIAP1/2/3/4/5/6/7/8/9TEMP	
2	Run FUNC-DCU-04-PHOT test procedure from the CCS	
5	Contingency: If test fails repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-04-PHOT	SCUDCDCSTAT PLIAP5V PLIAP9V PLIAM9V LIAP1TEMP to LIAP9TEMP	4/5 0/~ +5V 0/~+11V 0/~-11V N/A/ [290-300]K	4/5 0/+5.23V 0/+11.58V 0/-11.58V ~293/warming up		Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 54 of 105

Start time: 11:19

OBSID: 0xb00002d0

CUS Input Default Parameters:

`int mcu_status = 1; //default 0 = off, 1= on`

Comments: PLIABITSTAT 0 to 1

Photometer LIAs switched on OK

Output file FUNC-DCU-04p_B00002D0.txt from QLA script:

DCU-04-phot
Start time @: 23-Oct 11:20:08
End time @: 23-Oct 11:20:22
OBSID: 0xB00002D0

PLIABITSTAT:
Start value: OFF
End value: 1.0

	Before/After
SCUDCDCSTAT	4/5
PLIAP5V	0.22/5.23 V
PLIAP9V	0.02/11.58 V
PLIAM9V	0.02/-11.58 V


QLA plots below for Phot LIA temperatures



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 55 of 105

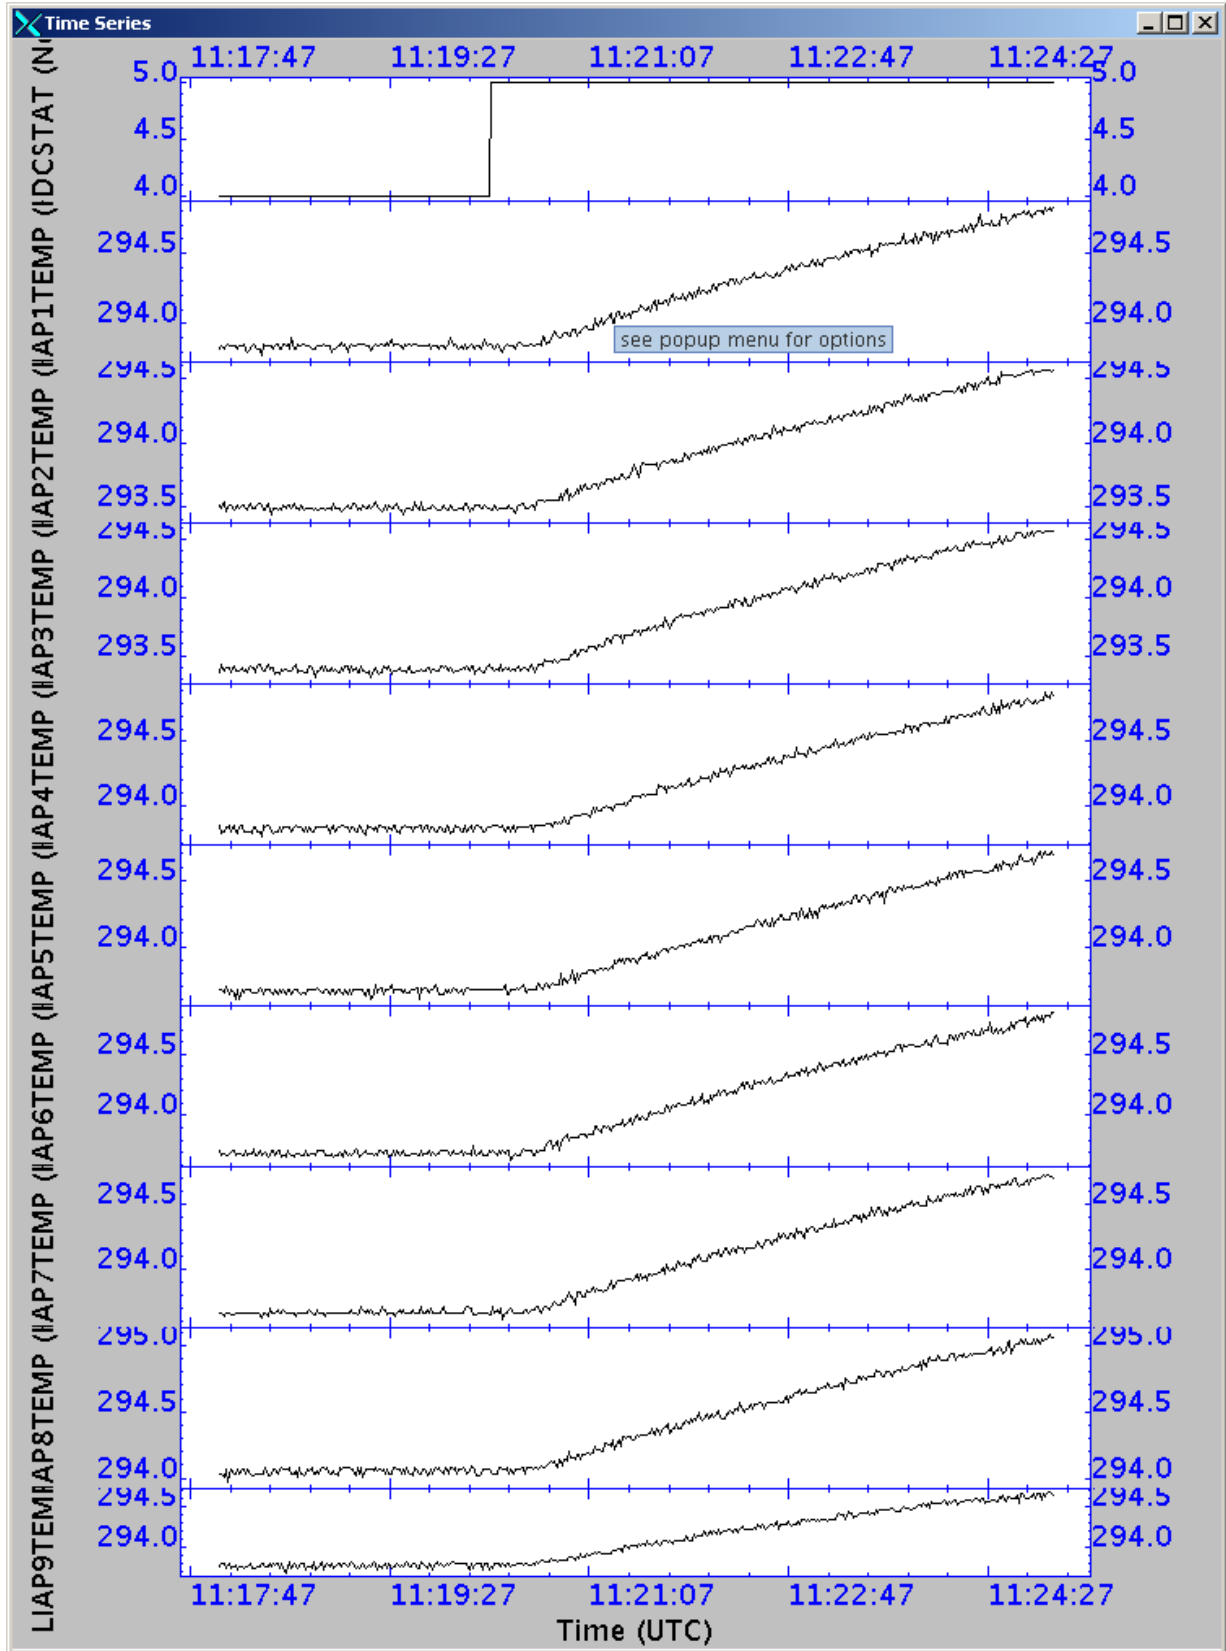



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	56 of 105

4.24 FUNC-DCU-11-PHOT: Photometer BDAs Switch ON Check

Test Id:	FUNC-DCU-11-PHOT: Photometer BDAs Switch ON Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ Photometer LIAs ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ Photometer LIAs ON + Photometer BIAS ON +Photometer JFETs ON
Success Criteria:	Test passed if Photometer JFET source and drain voltages are as commanded: <ol style="list-style-type: none"> 1. PSWJFETVSS1/2/3/4/5/6 2. PMLWJFETVSS1/2/3/4 3. PSWJFETSTAT = 0x3F 4. PMLWJFETSTAT = 0x7F

Test Procedure:

Step#	Action	Comments
1	Run FUNC-DCU-11-PHOT test procedure	
2	After the test Write the values RAW and converted values of: PSWJFETSTAT,PMLWJFETSTAT, PSWJFET1/2/3/4/5/6V PMWJFET1/2/3/4V PLWJFET1/2V located in DCU PARAMETERS AND	
3	Contingency: If test fails repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-11P	PSWJFETSTAT PMLWJFETSTAT PSWJFET1/2/3/4/5/6V PMWJFET1/2/3/4V PLWJFET1/2V	0/0x3f 0/0x7f 0V/-1.5V 0V/~-1.5V 0V/~-1.5V	0/0x03f 0/0x07f See comments	N/A	Pass



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 57 of 105

Start time: 11:22

OBSID: 0xb00002d1

CUS Input Default Parameters:

int heater_V = 0; // Specifies if the heater is to be switched ON or not
string array = "PF"; //default array to switch ON

Comments:

The Vss values were the ~ -1.5V, as agreed with SPIRE instrument team, i.e.

PSWJFET1V: -1.47V

PSWJFET2V: -1.47V

PSWJFET3V: -1.47V

PSWJFET4V: -1.47V

PSWJFET5V: -1.47V

PSWJFET6V: -1.47V

PMWJFET1V: -1.47V

PMWJFET2V: -1.47V

PMWJFET3V: -1.47V

PMWJFET4V: -1.47V

PLWJFET1V: -1.47V

PLWJFET2V: -1.47V

TCJFETV: -1.47V

**The PSW, PMW and PLW arrays on QLA are all OK
DCU data were generated for ~1min after JFET switch on.
QLA produced output file FUNC-DCU-11p_B00002D1.txt:**

DCU-11-phot

Start time @: 23-Oct 11:24:10

End time @: 23-Oct 11:25:59

OBSID: 0xB00002D1

PLIABITSTAT:

Start value: 0x0

End value: 0x4C

Before/After

PSWJFETSTAT 0x0/0x3F

PMLWJFETSTAT 0x0/0x7F

PSWJFET1V -0.00/-1.47 V

PSWJFET2V -0.00/-1.47 V

PSWJFET3V -0.00/-1.47 V

PSWJFET4V -0.00/-1.47 V

PSWJFET5V -0.00/-1.47 V

PSWJFET6V -0.00/-1.47 V

PMWJFET1V -0.00/-1.47 V

PMWJFET2V -0.00/-1.47 V

PMWJFET3V -0.00/-1.47 V

PMWJFET4V -0.00/-1.47 V

PLWJFET1V -0.00/-1.47 V

PLWJFET2V -0.00/-1.47 V

TCJFETV 0.00/-1.47 V



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	58 of 105

4.25 FUNC-DCU-13-PHOT: Photometer BDAs Integrity Check

Test Id:	FUNC-DCU-13P: Photometer BDAs Integrity Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ Photometer LIAs ON + Photometer BIAS ON +Photometer JFETs ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ Photometer LIAs ON + Photometer BIAS ON +Photometer JFETs ON
Success Criteria:	Test passed if : The photometer detectors show a small linear variation on the output voltage when different bias is applied through the load curve.

Test Procedure:

Step#	Action	Comments
1	On QLA bring up a time series display of a couple of pixels on each of the photometer BDAs	
2	Run FUNC-DCU-13-PHOT test procedure from the CCS	
3	Contingency: If test fails repeat step 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-13-PHOT				N/A	Success



Start time: 11:37

OBSID: 0xb00002d2

CUS Input Default Parameters:

```
string dcumode = "PF"; // Specifies array in which to perform LC
int mclkdiv = 0x95; // Master clock divisor ,which specifies bias freq
int biasdiv = 0x6; // Sampling divisor ,which specifies sampling rate
int psw_phase = 0x80; // PSW demod phase
int pmw_phase = 0x80; // PMW demod phase
int plw_phase = 0x80; // PLW demod phase
int ftime = 10; // Time at each bias level
```

– Took ~2 minutes to receive all the TC stream from the I-EGSE from the start of execution from the CCS

Comments: Most pixels look better than or the same as in PFM5 ILT

1) Pixels which showed correct polarity in PFM5 ILT but which now show wrong polarity are:

PSW-D15

PTC3

NCR HP-112000-ASED-NC-3734 raised.

2) Pixels which showed anomalous behaviour in PFM5 ILT and which now show wrong polarity are:

PMW-B6

3) Pixels which showed wrong polarity in PFM5 ILT and which still show wrong polarity are:

PMW-F7

4) Pixels which showed wrong polarity or anomalous behaviour in PFM5 ILT but which now show correct polarity or normal behaviour are:

PSW-A10

PSW-F8

PSW-G13

PMW-C8

PMW-D7

PMW-E10

PMW-DP1

PMW-T2

PMW-G11

PLW-B4

PLW-A2

PLW-DP1

QLA load curve plots in Annexe 2.



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	60 of 105

Photometer detector settings at the end of the test:

Bias F: ~130.2 Hz

Samp F: 18.6 Hz

Phases: all ~180.7

Biases are ~31mV,

TC BIAS: ~61mV



4.26 FUNC-DCU-14-PHOT: Photometer BDAs Noise Check

Test Id:	FUNC-DCU-14-PHOT: Photometer BDAs Noise Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Photometer LIAs ON + Photometer BIAS ON + Photometer JFETs ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Photometer LIAs ON + Photometer BIAS ON + Photometer JFETs ON
Success Criteria:	Test passed if : The Photometer detectors don't show excess noise.

Test Procedure:

Step#	Action	Comments
1	Run FUNC-DCU-14-PHOT test procedure from the CCS	
2	Contingency: If test fails repeat step 1.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-14-PHOT				N/A	Success

Start time: 12:08
OBSID: 0xb00002d3

CUS Input Default Parameters:
string dcumode = "PF"; //Array
int ftime = 120; //time

Comments: Test OK
Detectors settings:
 Bias frequency: 130.2Hz
 Sampling frequency: 18.6 Hz
 PSW phase: 180.71 deg
 PMW phase: 180.71 deg
 PLW phase: 180.71 deg
 PSW bias : ~ 31mV
 PMW bias : ~ 31mV
 PLW bias : ~ 31mV
 TC bias : ~ 62 mV

Duration of test: 2 minutes




QLA plots below (one pixel per array)



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 62 of 105

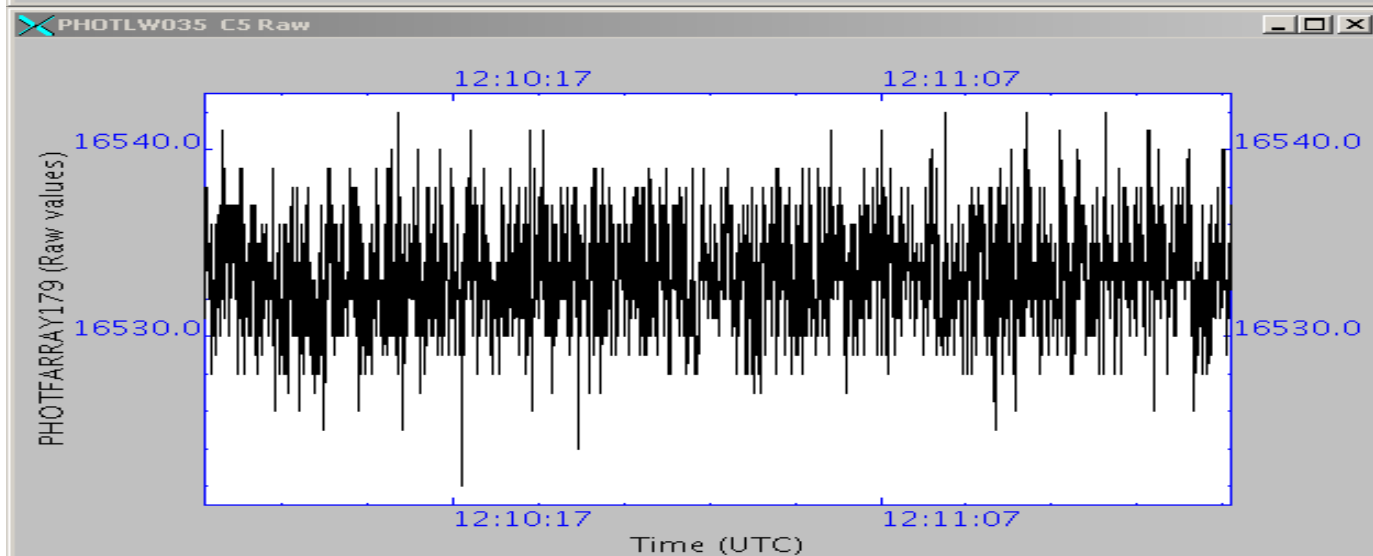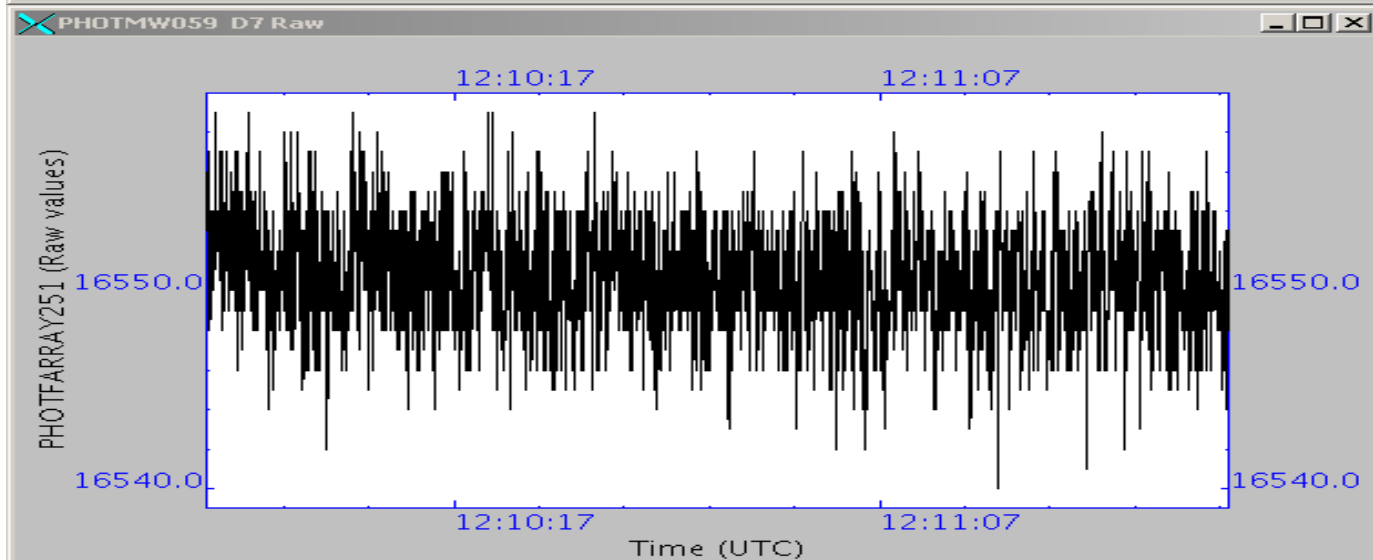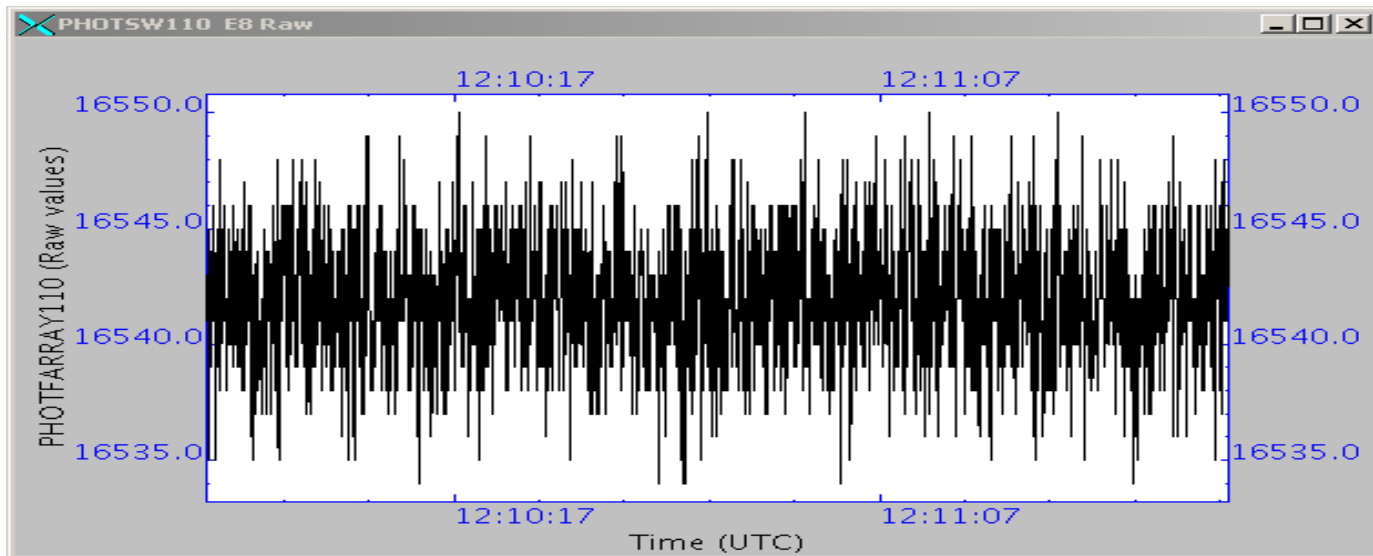



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
 Prime Side
 S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 63 of 105

Switched off the Photometer:

PDET_OFF: 0xb00002d4

Start time: 12:13

4.27 FUNC-DCU-04-SPEC: Spectrometer LIAs Check

Test Id:	FUNC-DCU-04-SPEC: Spectrometer LIAs Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Spectrometer LIAs ON
Success Criteria:	Test passed if : <ol style="list-style-type: none"> SCUDCDCSTAT parameter goes from 4 to 6. Spectrometer LIA card voltages are showing correct readings of +5V,+9V,-9V. Spectrometer LIA temperatures show an increase indicating that they are ON.

Test Procedure:

Step#	Action	Comments
1	On QLA bring up a time series display of the HK parameters: SLIAP5V SLIAP9V SLIAM9V LIAS1/2/3TEMP	
2	Run FUNC-DCU-04-SPEC test procedure from the CCS	
5	Contingency: If test fails repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-04-SPEC	SCUDCDCSTAT SLIAP5V SLIAP9V SLIAM9V LIA1/2/3TEMP	4/6 0/~ +5V 0/~+11V 0/~-11V N/A/ [290-300]K	4/6 0.11 / 5.25 0.016/ 11.59 0.016/-11.56 /~296-297K warming up		Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 64 of 105

Start time: 12:14

OBSID: 0xb00002d5

CUS Input Default Parameters:

int mcu_status = 1; //default 0 = off, 1= on

Comments: SLIABITSTAT 0 to 1

Spectrometer LIAs switched ON correctly

Output file FUNC-DCU-04s_B00002D5.txt from QLA script:

DCU-04-spec

Start time @: 23-Oct 12:21:02

End time @: 23-Oct 12:22:42

OBSID: 0xB00002D6


SLIABITSTAT:

Start value: ON

End value: 1.0

	Before/After
SCUDCDCSTAT	6/6
SLIAP5V	5.25/5.25 V
SLIAP9V	11.59/11.59 V
SLIAM9V	-11.56/-11.56 V

QLA plots below for Spec LIA temperatures

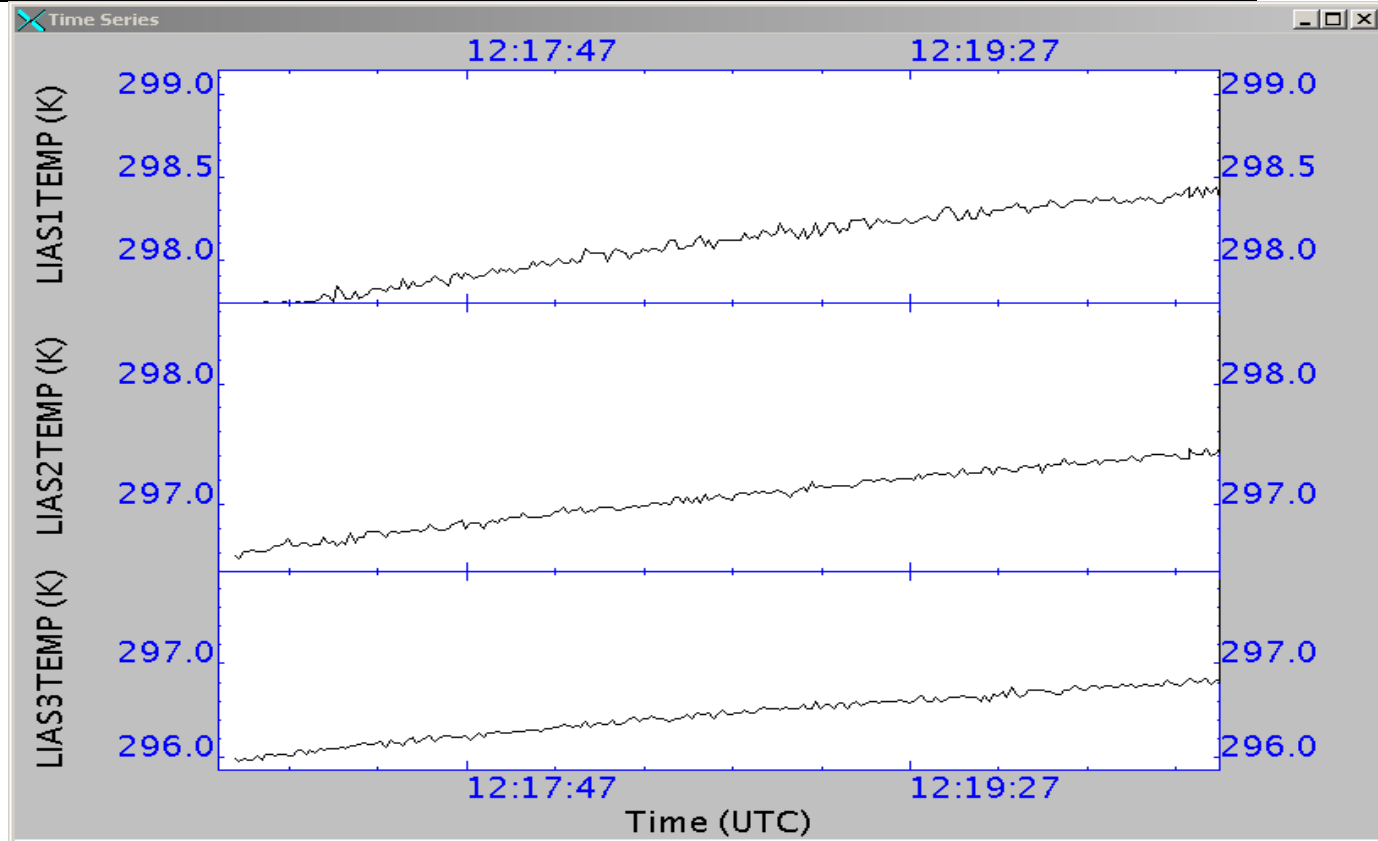



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	65 of 105

4.28 FUNC-DCU-11-SPEC: Spectrometer BDAs Switch On Check

Test Id:	FUNC-DCU-11-SPEC: Spectrometer BDAs Switch On Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Spectrometer LIAs ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Spectrometer LIAs ON + Spectrometer BIAS ON + Spectrometer JFETs ON
Success Criteria:	Test passed if SCUDCDCSTAT goes from 4 to 6, Spectrometer LIAs voltages are correct and SJFET voltages are also correct.

Test Procedure:

Step#	Action	Comments
1	Run FUNC-DCU-11-SPEC test procedure from the CCS	
2	After the test Write the values RAW and converted values of: LIASTAT SLIAP5V, SLIAP9V, SLIAM9V, SSWJFETSTAT,SLWJFETSTAT, SSWJFET1V,SLWJFET2V located in DCU PARAMETERS AND	
3	Contingency: If test fails repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-11-SPEC	SCUDCDCSTAT LIASTAT SLIAP5V SLIAP9V SLIAM9V SPECJFETSTAT SSWJFET1/2V SLWJFET1/2V	6/6 0/0 0V/ ~ 5V 0V/~11V 0V/~11V 0/0x7 0V/~-1.5V 0V/~-1.5V	6/6 0/0 /5.25 /11.59 /-11.59 0/0x7 See comments below	N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 66 of 105

Start time: 12:19

OBSID: 0xb00002d6

CUS Input Default Parameters:

int heater_V = 0; // Specifies if the heater is to be switched ON or not
string array = "SF"; //default array to switch ON

Comments:

The Vss values were the ~ -1.5V, as agreed with SPIRE instrument team, i.e.

SSWJFET1V: -1.47V

SSWJFET2V: -1.47V

SLWJFET1V: -1.47V

QLA produced file FUNC-DCU-11s_B00002D6.txt:

DCU-11-spec

Start time @: 23-Oct 12:21:00

End time @: 23-Oct 12:22:42

OBSID: 0xB00002D6

SLIABITSTAT:

Start value: 0x1

End value: 0x1

	Before/After
SCUDCDCSTAT	0x6/0x6
LIASAT	0x0/0x0
SLIAP5V	5.25/5.25 V
SLIAP9V	11.59/11.59 V
SLIAM9V	-11.56/-11.56 V
SPECJFETSTAT	0x0/0x7
SSWJFET1V	-0.00/-1.47 V
SSWJFET2V	-0.00/-1.47 V
SLWJFET1V	-0.00/-1.47 V



4.29 FUNC-DCU-13-SPEC: Spectrometer BDAs Integrity Check

Test Id:	FUNC-DCU-13-SPEC: Spectrometer BDAs Integrity Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Spectrometer LIAs ON + Spectrometer BIAS ON + Spectrometer JFETs ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Spectrometer LIAs ON + Spectrometer BIAS ON + Spectrometer JFETs ON
Success Criteria:	Test passed if : The spectrometer detectors show a small linear variation on the output voltage when different bias is applied through the load curve.

Test Procedure:

Step#	Action	Comments
1	Run FUNC-DCU-13-SPEC test procedure from the CCS	
2	Contingency: If test fails repeat step 1.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-13-SPEC				N/A	Success



**Start time: 12:24 -
OBSID: 0xb00002d7**

CUS Input Default Parameters:

```
string dcumode = "SF"; //DCU data mode
int mclkdiv = 0x79; //Master clock divisor
int biasdiv = 0x1; // Bias divisor
int ssw_phase = 0x80; // SSW demod phase
int slw_phase = 0x80; // SLW demod phase
int ftime = 10; // Time at each bias level
```

Comments: – Took ~2 minutes to receive all the TC stream from the I-EGSE from the start of execution from the CCS

Generally all (SSW/SLW) pixels looking responsive. All pixels look better than or same as for PFM5 ILT

Comments: Most pixels look better than or the same as in PFM5 ILT

Pixels which showed wrong polarity or anomalous behaviour in PFM5 ILT but which now show correct polarity or normal behaviour are:

**SLW-C2
SLW-DP2
SLW-B3
SLW-C4
SLW-T2**

See Annexe 2 for detailed results.



4.30 FUNC-DCU-14-SPEC: Spectrometer BDAs Noise Check

Test Id:	FUNC-DCU-14S: Spectrometer BDAs Noise Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Spectrometer LIAs ON + Spectrometer BIAS ON + Spectrometer JFETs ON
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON + Spectrometer LIAs ON + Spectrometer BIAS ON + Spectrometer JFETs ON
Success Criteria:	Test passed if : The spectrometer detectors show a signal with some noise.

Test Procedure:

Step#	Action	Comments
1	Run FUNC-DCU-14-SPEC test procedure from the CCS	
2	Contingency: If test fails repeat step 1.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-DCU-14-SPEC				N/A	Success

Start time: 12:38
OBSID: 0xb00002d8

CUS Input Default Parameters:
string dcumode = "PF"; //Array
int ftime = 120; //time

Comments:

Test run in order to collect noise data at nominal spectrometer settings:

Array: SF
Bias frequency: 160 Hz
Sampling frequency: 80 Hz
SSW phase shift: ~180.71 deg
SLW phase shift: ~180.71 deg

Duration of test: 5 minutes



QLA plots below (one pixel per array)



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 70 of 105

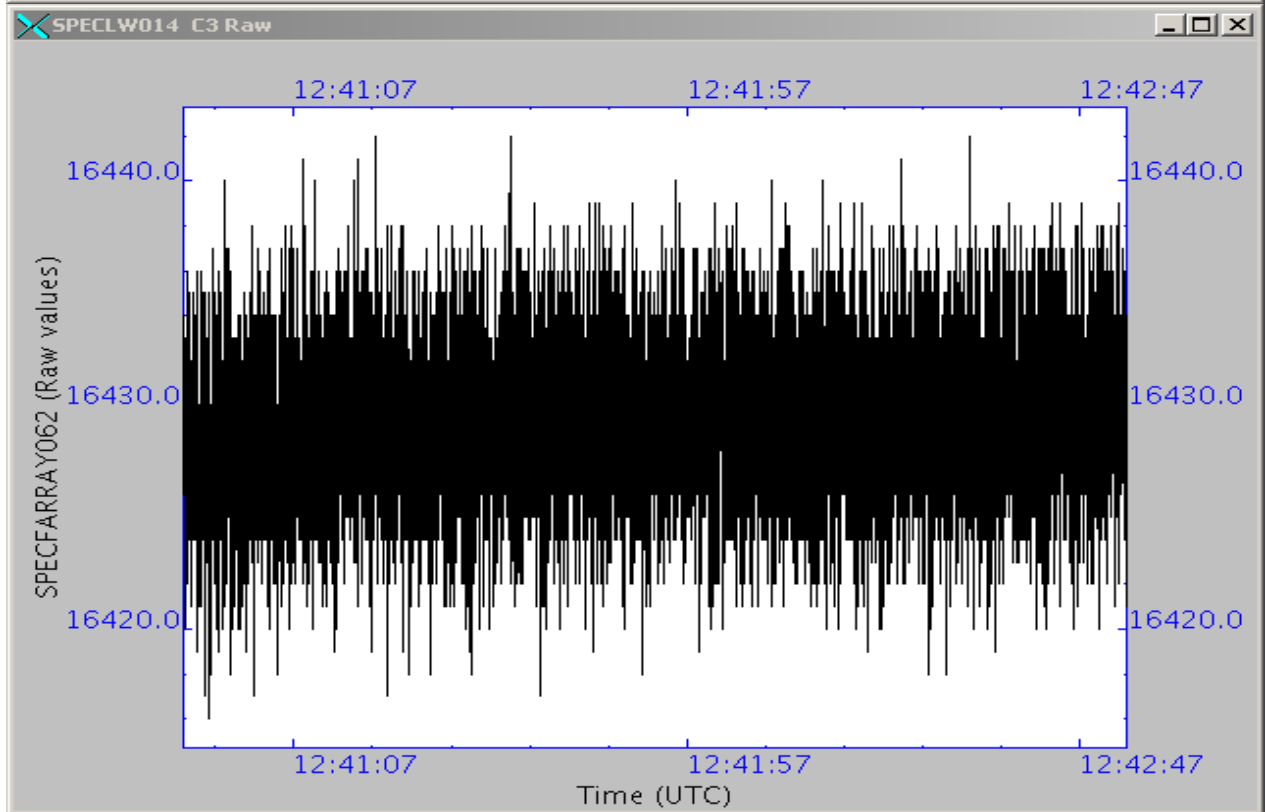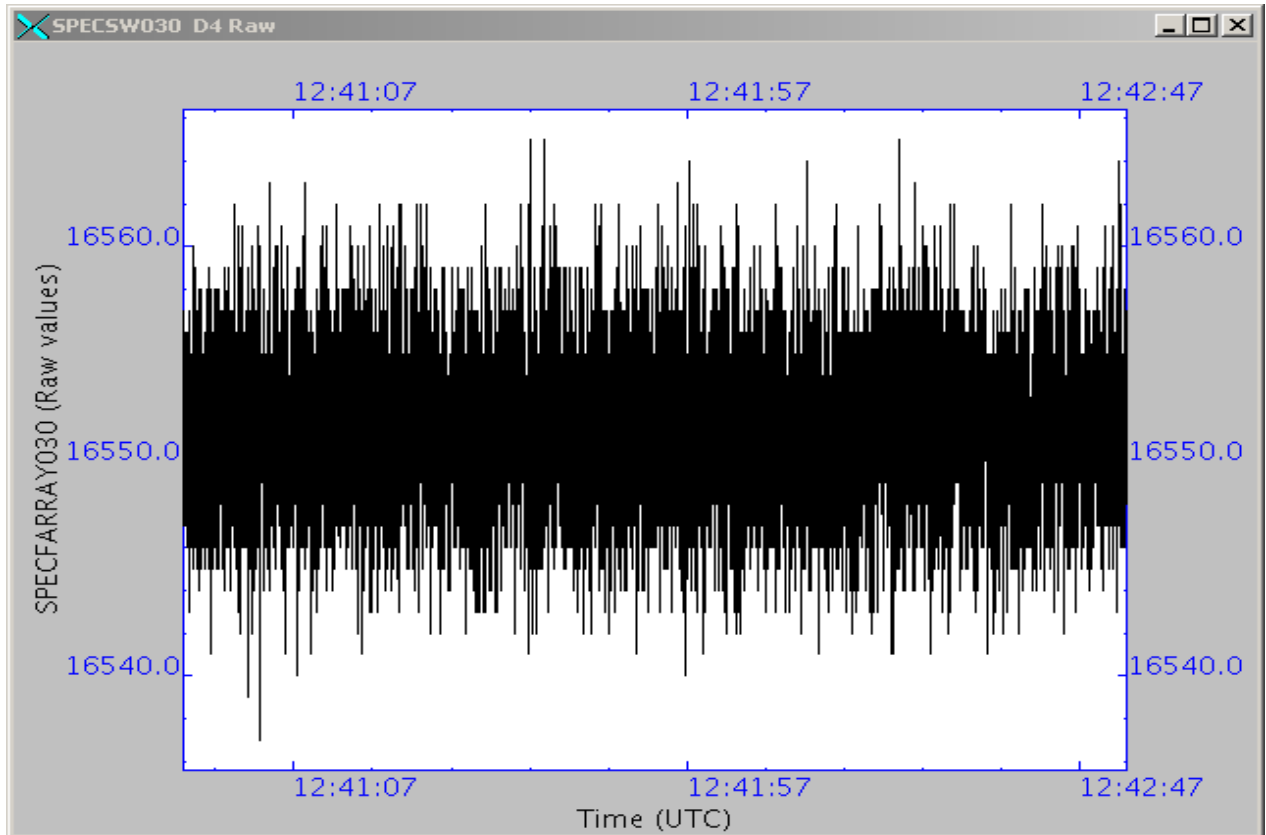



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
 Prime Side
 S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 71 of 105

Switched off the Spectrometer:
 SDET_OFF: 0xb00002d9
 Start time: 12:48

4.31 FUNC-SMEC-01: SMEC Encoder and LVDT Check

Test Id:	FUNC-SMEC-01: SMEC Encoder and LVDT Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON+ SMEC ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON+ SMEC ON (open loop)
Success Criteria:	Test passed if : <ol style="list-style-type: none"> SMECENCPWR HK parameter changes from 0 to 6. SMEC encoder signals 1 and 2 show variation when encoder is switched ON. SMEC LVDT is switched ON. SMEC LVDT DC and AC signals show variation when LVDT is switched ON.

Test Procedure:

Step#	Action	Comments
0	Open SMEC PARAMETERS display on SCOS Alpha Numeric Displays.	
1	On QLA bring up a display of the following HK parameters: SMECENCPWR SMECENC SIG1AMP SMECENC SIG2AMP SMECLVDTDCSIG SMECLVDTACSIG	
2	Run FUNC-SMEC-01 test procedure from the CCS	
	Contingency: If test fails repeat steps 1.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/ After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SMEC-01	SMECENCPWR SMECLVDPWR SMECENC SIG1 SMECENC SIG1AMP SMECENC SIG1OFF SMECENC SIG2 SMECENC SIG2AMP SMECENC SIG2OFF	0/6 0/1 Changes 0/0 -/0x57E4 Changes 0/0 -/0x6D60	0/6 0/1 ~0x3079/~0x54c1 0/0 0xCE20/0x57E4 ~0x4E6B/~0x6534 0/0 0xCE20/0x6D60	N/A	Success



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King


Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 72 of 105

Start time: 12:52
OBSID: 0xb00002da

CUS Input Default Parameters:

string smec_temp = "warm"; //(cold/warm) Used to specify the encoder power level

Comments:

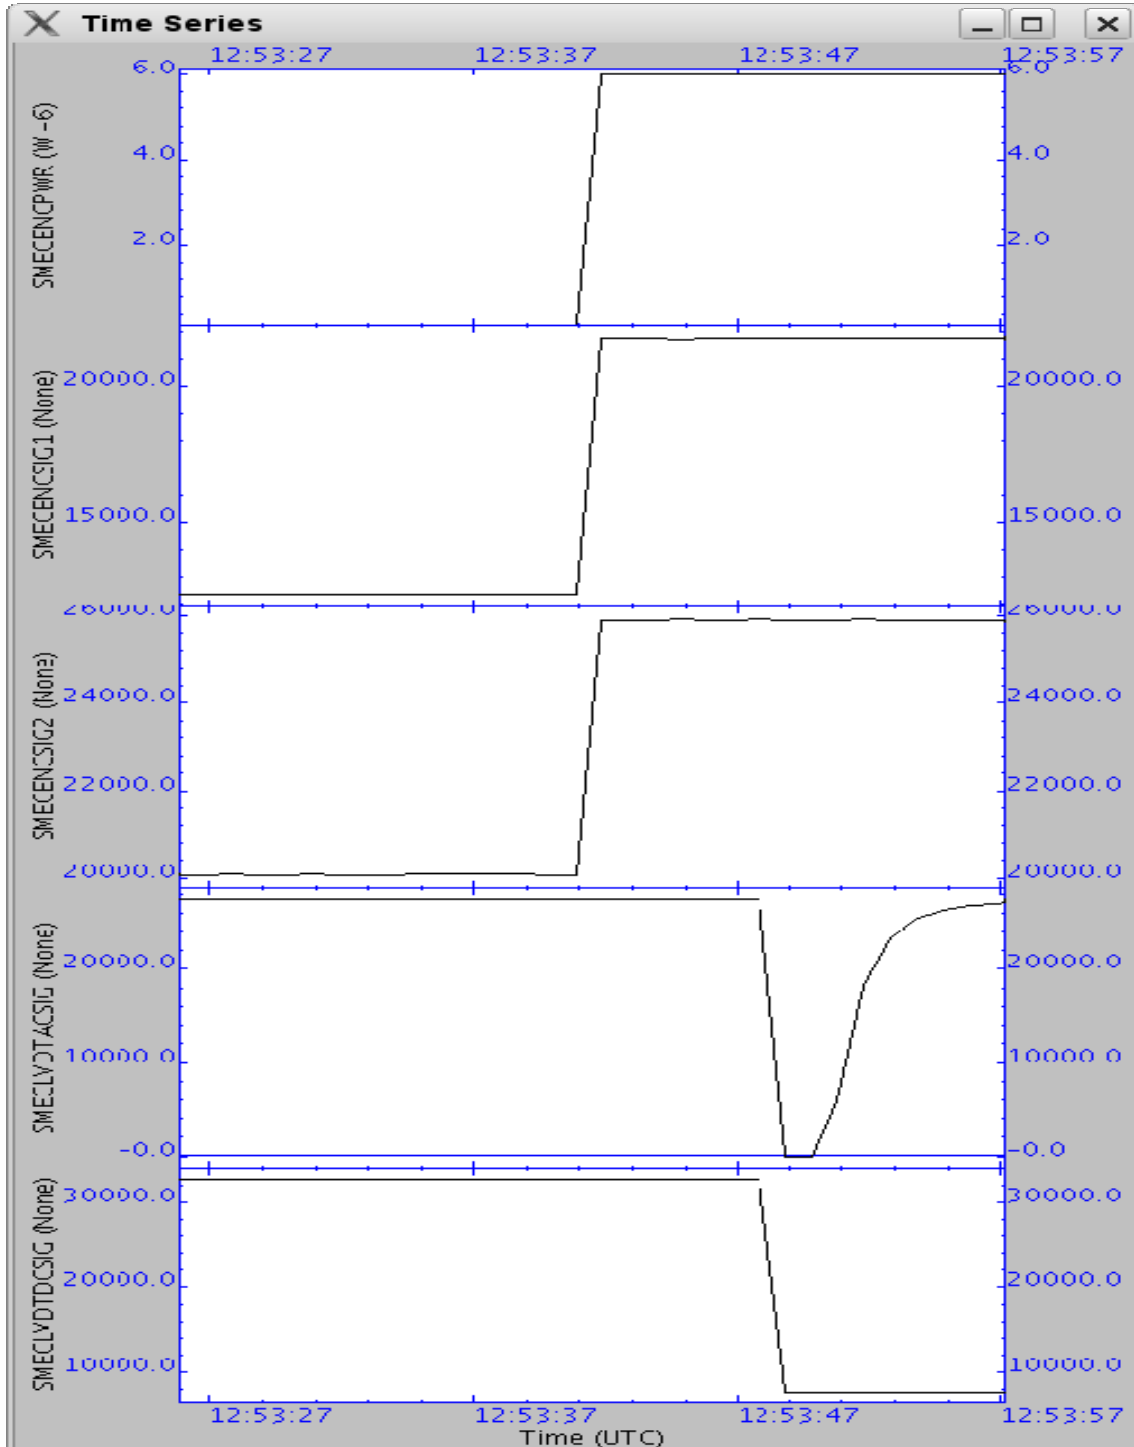



4.32 FUNC-SMEC-03: SMEC Encoder Levels Check

Test Id:	FUNC-SMEC-03: SMEC Encoder Levels Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON+ SMEC ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON+ SMEC ON (open loop)
Success Criteria:	Test passed if: SMEC encoder signals 1 and 2 show a variation on their amplitudes from one LED illumination level to another.

Test Procedure:

Step#	Action	Comments
1	On QLA bring up a time series display of the following Nominal HK parameters: SMECENC SIG1 SMECENC SIG2	
2	Run FUNC-SMEC-03 test procedure from the CCS	
3	Contingency: If test fails repeat steps 1 and 2.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SMEC-03	SMECENC SIG1 SMECENC SIG2	Signals change with LED levels	See below		Success

Start time: 13:00
OBSID: 0xb00002db

CUS Input Default Parameters:

```
string frametype = "ENG"; // Specifies MCU frame type
double framerate = 64.0; // Specifies the frame rate
int framenum = 0xffff; // Frame number
int level_init = 6; //
int level_start = 4;
int level_end = 6;
int level_step = 1;
int led_delay = 5; // Time at each level in seconds
```

Comments:

LED Level	SMECENC SIG1	SMECENC SIG2
4	~14800	~22000
5	~17000	~23200
6	~21700	~25800



4.33 FUNC-SMEC-02A: SMEC Open Launch Latch

Test Id:	FUNC-SMEC-02A: SMEC Open Launch Latch
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + SMEC ON SMEC Latched
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + SMEC ON SMEC Unlatched
Success Criteria:	Test passed if : Prior to un-latching the resistance across pins 7 and 8 of the launch latch is ~ 368 Ohms. After un-latching the resistance is 483 Ohms. Note: These resistance values were recorded for the CQM SMEC model, for the flight SMEC, these values are expected to vary.

Step#	Action	Comments
1	Measure the resistance across pins 7 and 8 of the launch latch.	This step is not applicable anymore
2	Run FUNC-SMEC-02A test procedure from the CCS	
3	Measure the resistance across pins 7 and 8 of the launch latch.	
4	Contingency: If test fails repeat steps 1.	

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SMEC-02A				N/A	See below



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	75 of 105

Start time: 13:13

OBSID: 0xb00002dc

CUS Input Default Parameters:

`string ltch = "latch"; // Command SMEC to unlatch`

Comments: It was ensured that the Herschel Cryostat was horizontal (+Y pointing upwards) for all tests which involved unlatching or moving the SMEC.

The script executed successfully but it cannot be confirmed at this stage if the SMEC is unlatched, as the SMEC was not moved.

Post Test Comment: After the tests it was discovered that the implementation of the SMEC Latch and Unlatch commands in the OBS is reversed. SPIRE System Problem Report SPR-629 has been raised.



4.34 FUNC-SMEC-04A: SMEC Open Loop Position Check

Test Id:	FUNC-SMEC-04A: SMEC Open Loop Position Check
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ SMEC ON (open loop) UNLATCHED
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ SMEC ON (open loop) UNLATCHED
Success Criteria:	Test passed if the SMEC parameters show variation indicating that the mechanism has moved.

Test Procedure:

Step#	Action	Comments
1	On QLA bring up a time series display of the following Nominal HK parameters: SMECENC SIG1 SMECENC SIG2 SMECLVDTDCSIG SMECLVDTAC SIG SMECMOTORCURRE	
2	Run FUNC-SMEC-04a test procedure from the CCS	
3	Contingency: If test fails repeat steps 1.	

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SMEC-04A					




Start time: 13:18
OBSID: 0xb00002dd

CUS Input Default Parameters:

```
string smec_temp = "warm"; //(cold/warm) Used to specify the encoder power level  
string frametype = "ENG"; // Specifies MCU frame type  
double framerate = 64.0; // Specifies the frame rate  
int scan_start = 1000 in [0,39900]; // Step look scan starting point (um)  
int scan_end = 15000 in [0,39900]; // Step look scan ending point (um)  
int scan_step = 1000 in [0,39900]; // Step look scan step size (um)  
int scan_fspeed = 500 in [0,2000]; // Scan forward speed (um/s)  
int scan_rspeed = 500 in [0,2000]; // Scan fly back speed (um/s)  
int ftime = 5; // Time at each target position in seconds
```

Comments: **The LVDT signal did not change and the SMEC encoder signal amplitudes are very small. Is the SMEC really unlatched?**

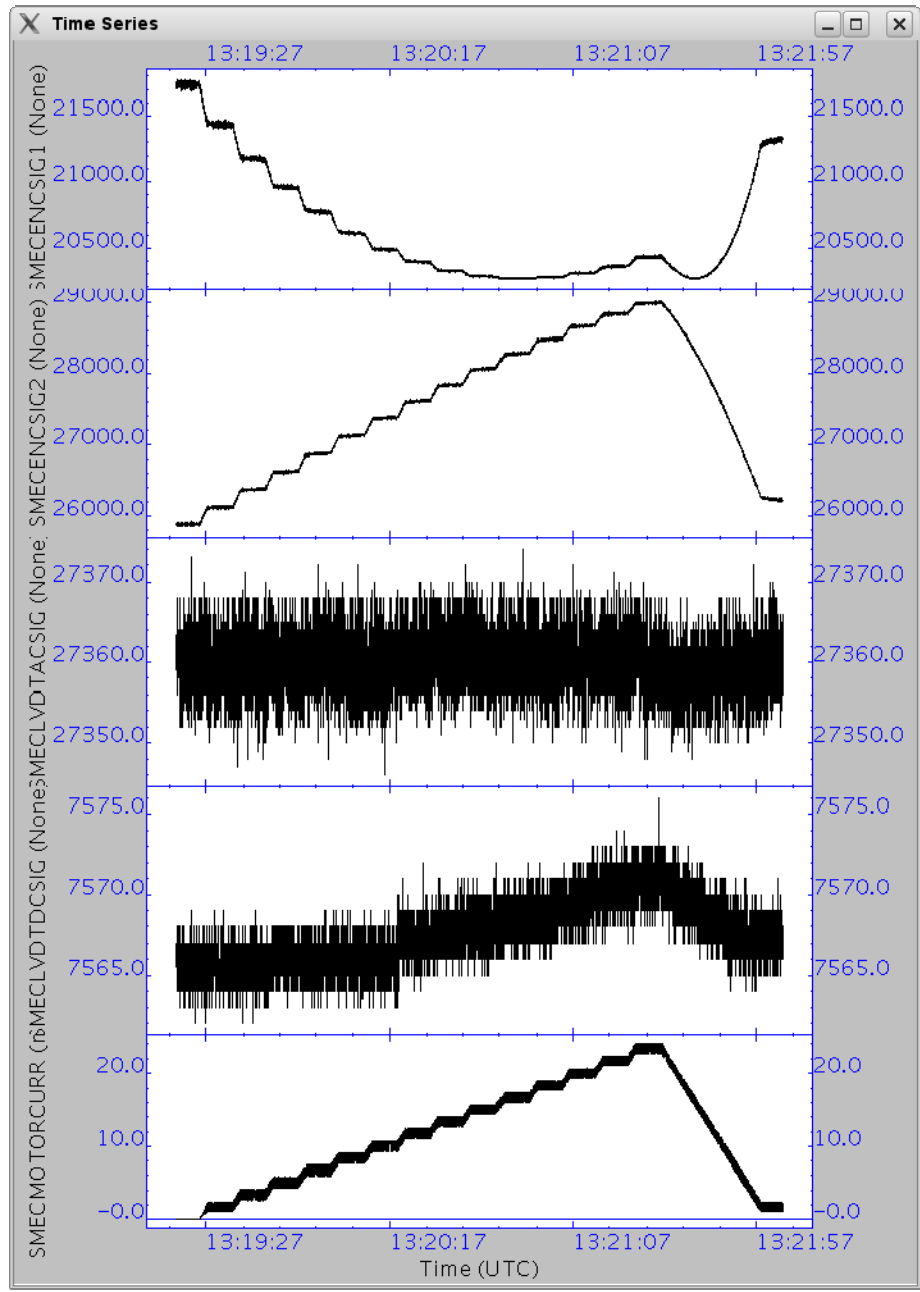



4.35 FUNC-SMEC-09: SMEC Open Loop Scan Check

Test Id:	FUNC-SMEC-09: SMEC Open Loop Scan Check
Test Purpose:	SMEC Open Loop Scan Test.
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ SMEC ON (open loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ SMEC ON (open loop)
Success Criteria:	Test passed if SMECLVDTDCSIG parameter shows a variation according to the different position of the SMEC along the scan.

Test Procedure:

Step#	Action
1	On QLA bring up a time series display of the following SMEC nominal science parameters: SMECENC SIG1 SMECENC SIG2 SMECLVDTDCSIG SMECLVDTACSIG SMECMOTORCURR
2	Run FUNC-SMEC-09 test procedure from the CCS
3	Contingency: If test fails repeat steps 1.

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	No. of frames received	Test Result
FUNC-SMEC-09	All above mentioned in step 2	N/A	N/A	N/A	Failed initially but see below



May need to set the SMEC encoder Sig1 & Sig2 offsets first

SIG1: 21300
SIG2: 26250


Start time: 13:35
OBSID: 0xb00002de

CUS Input Default Parameters:

```
string smec_temp = "warm"; //(cold/warm) Used to specify the encoder power level  
int scan_start = 1000 in [0,39900]; //Scan starting point (um)  
int scan_end = 15000 in [0,39900]; //Scan ending point (um)  
int scan_fspeed = 500 in [0,2000]; //Scan forward speed (um/s)  
int scan_rspeed = 500 in [0,2000]; //Scan reverse speed (um/s)  
int nscans = 2 in [2,65535]; //Number of scans (has to be even)  
double framerate = 64.0; // Specifies the frame rate
```

Comments:

The SMEC LVDT does not change with the SMEC motor current.

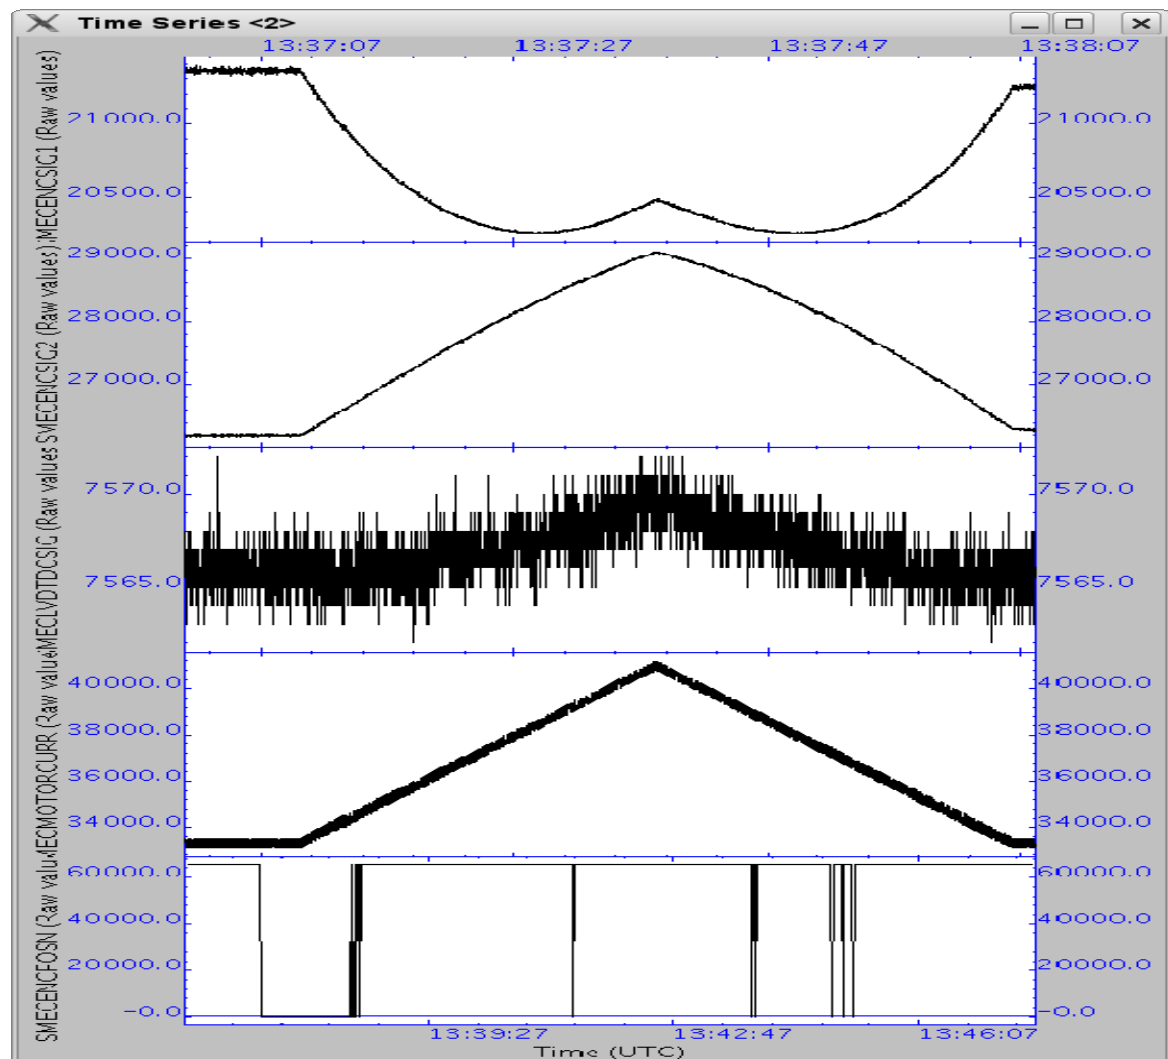



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	80 of 105

Run SMEC-02B to latch the mechanism:

Start time: 13:53
OBSID: 0xb00002df

The SMECMOTORCURR is 0x4DA4 – which corresponds to ~-39.3mA

16:12 – After talking to Dominique Pouliquen he suggests the following:

- **Set the FF offset to 0x7000**
16:17 0x90557000 The SMECMOTORCURR is ~-9.58mA
- **Release the latch manually:**
16:17 0x90430002
- **Run SMEC-04A:**
Start time: 16:19
OBSID: 0xb00002e0


The SMEC moved! See plot below. The LVDTDCSIG plot looks strange compared to last warm ILT.



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 81 of 105

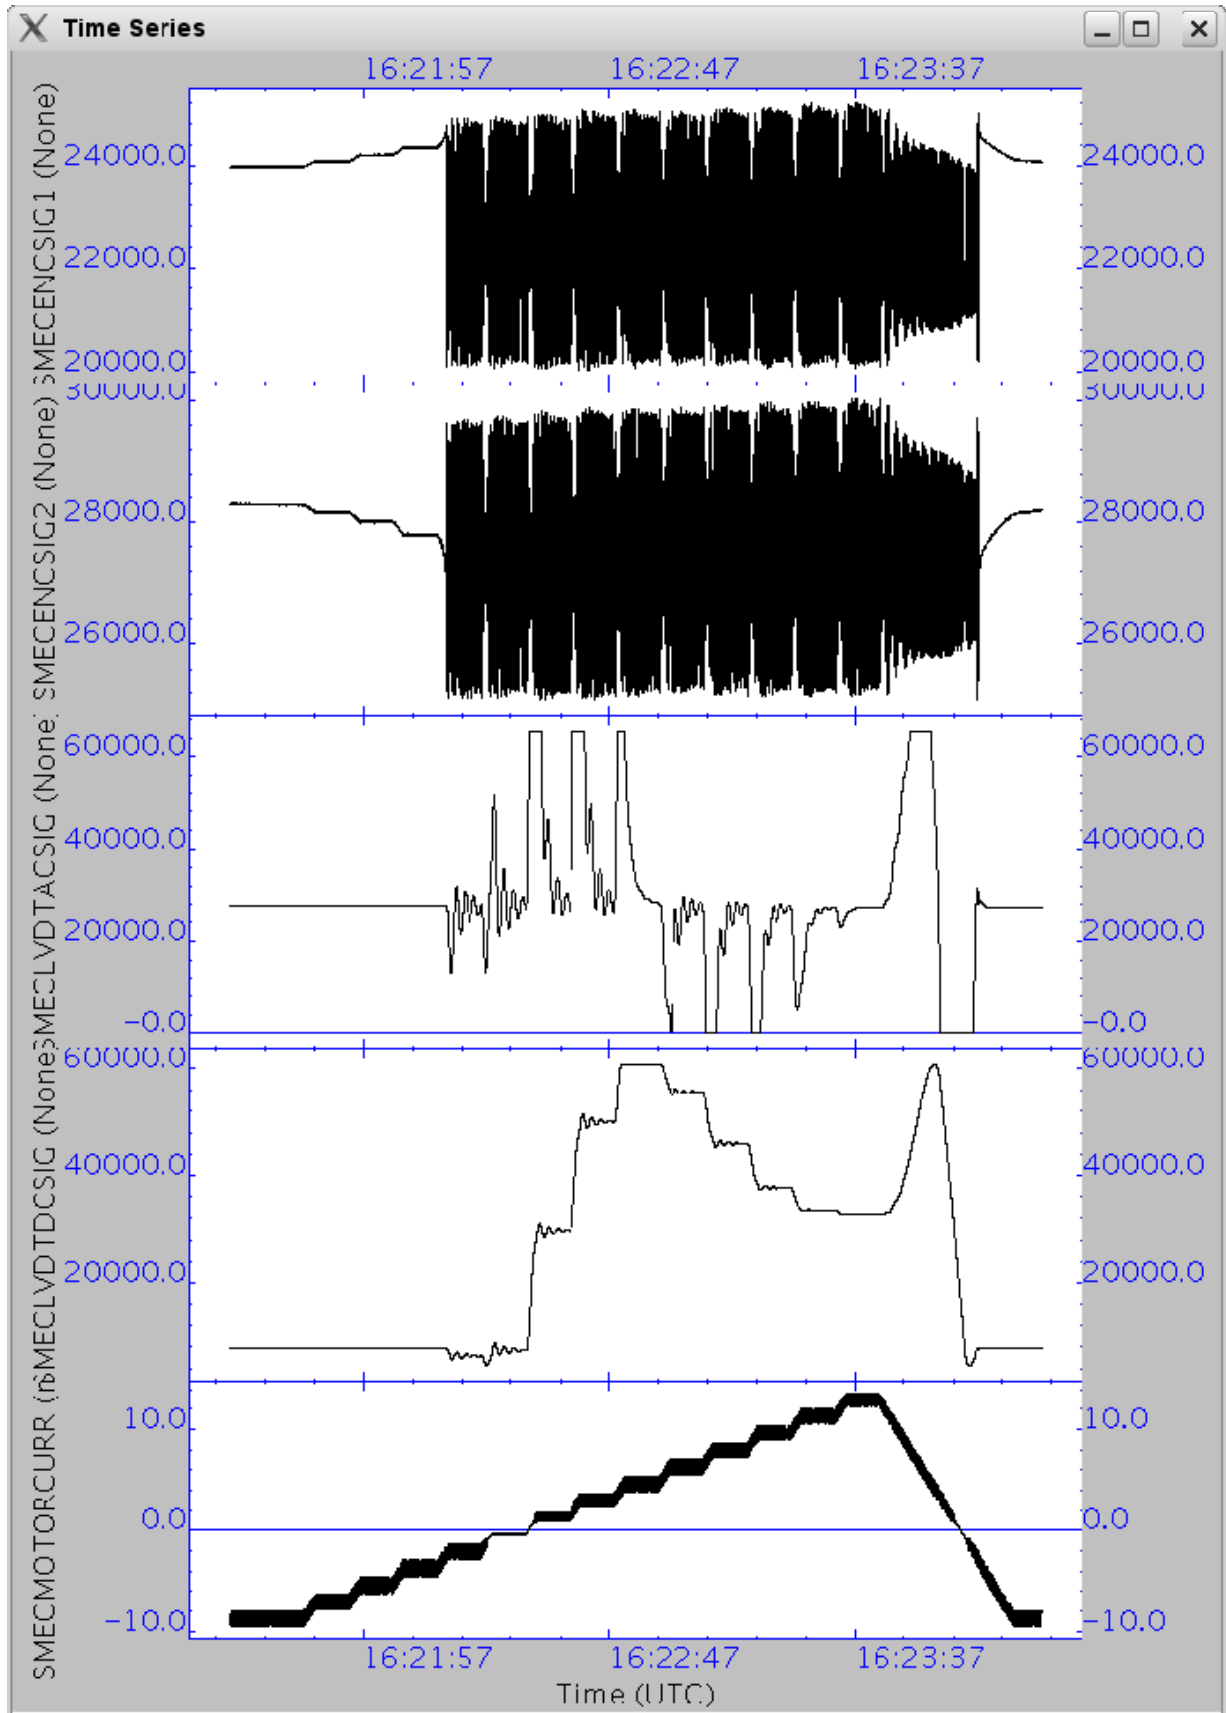



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	82 of 105

16:31 Set the encoder Signal 1 &2 offsets:

0x90585780

0x905a6b6c

FUNC-SMEC-09:

OBSID: 0xb00002e1


The SMEC scanning – **but the encoder signal amplitudes not optimum.**



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 83 of 105

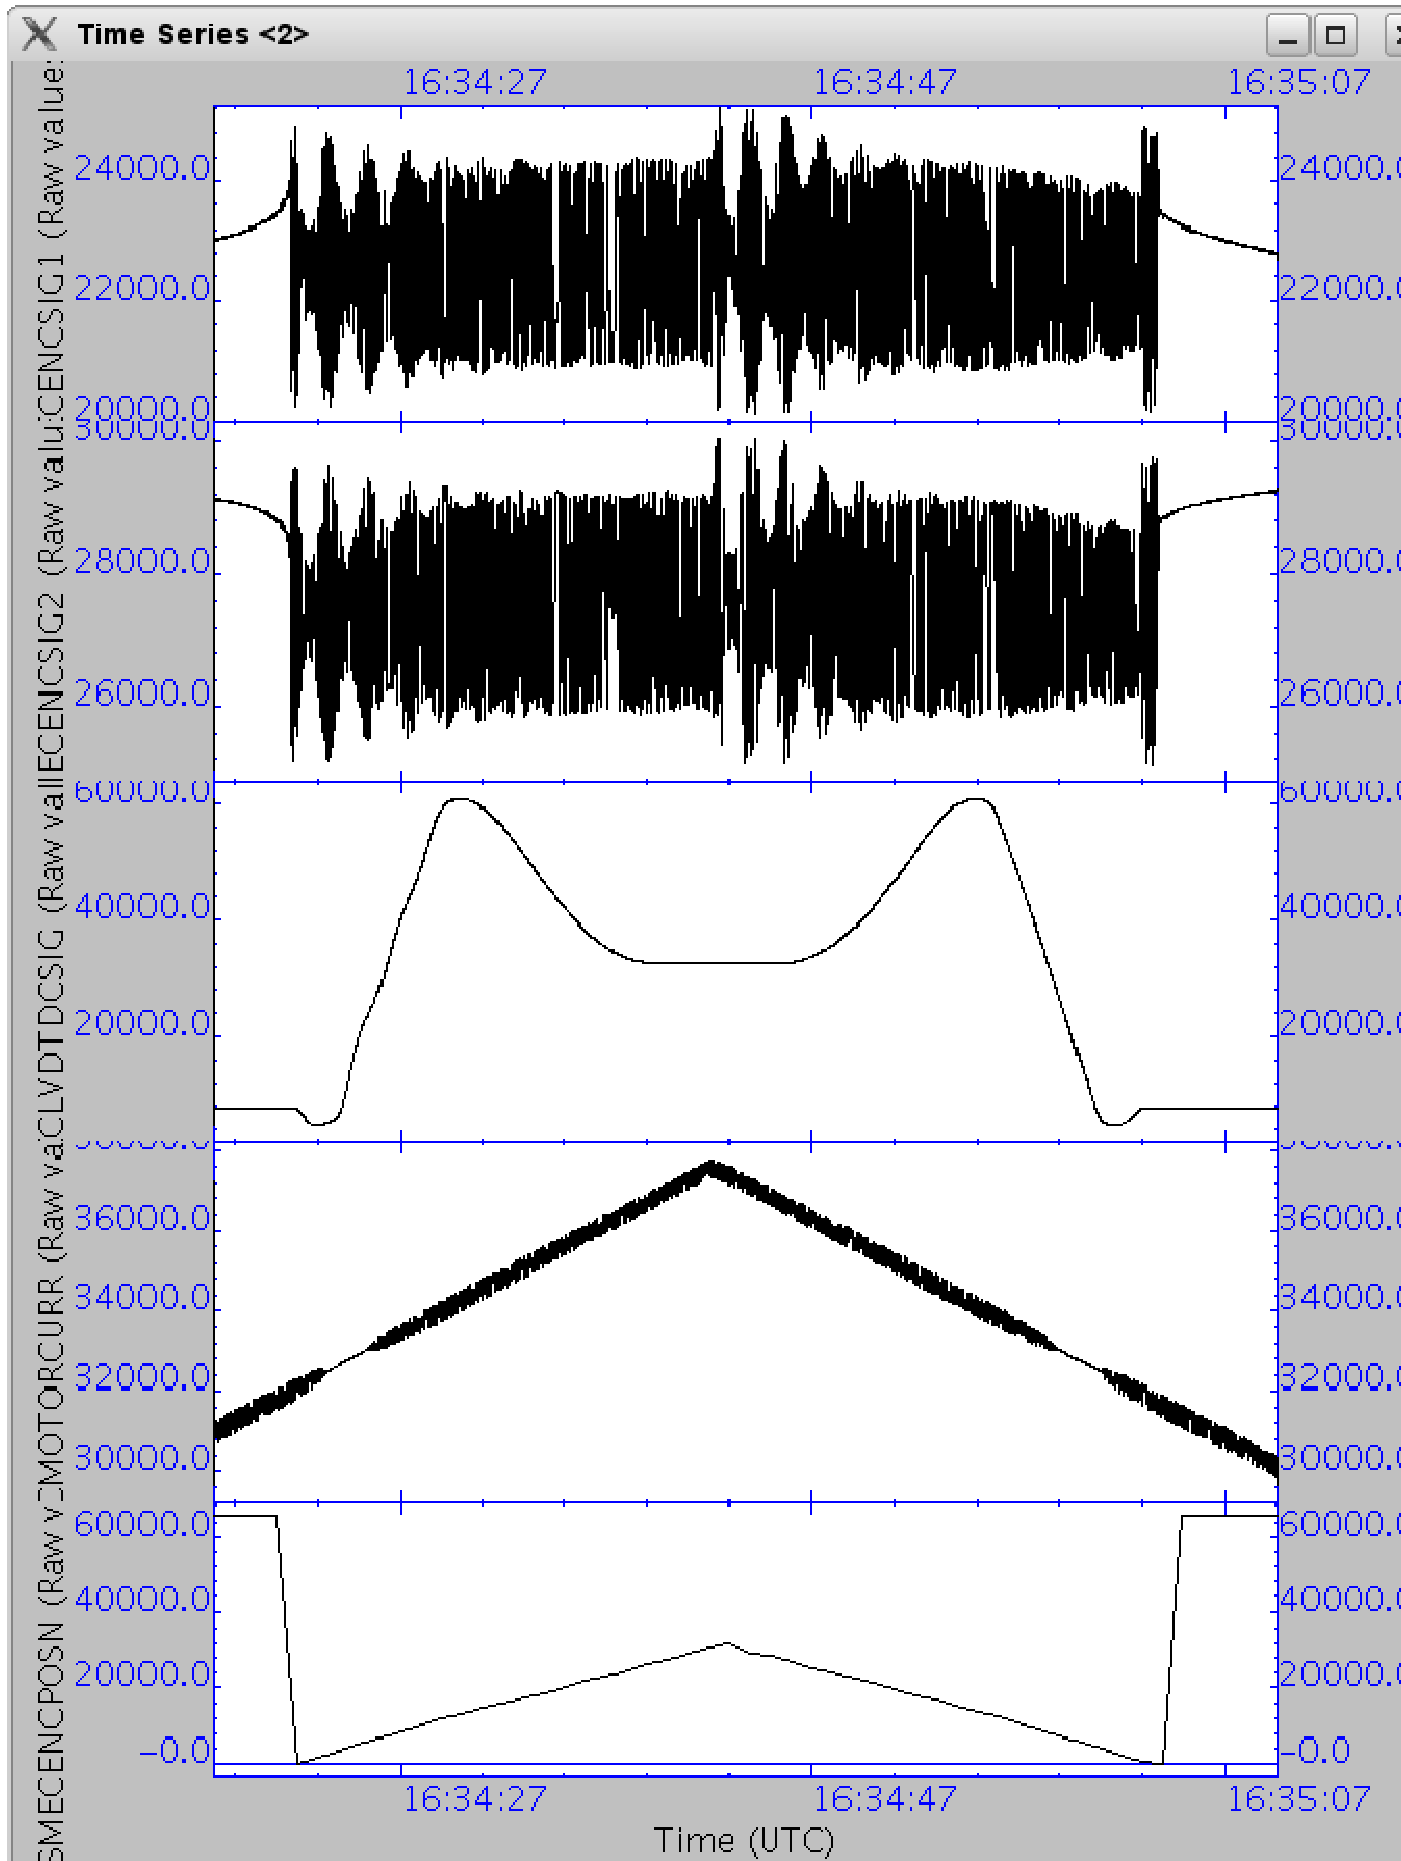



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	84 of 105

4.36 FUNC-SMEC-07: SMEC Closed Loop Scan Test

Test Id:	FUNC-SMEC-07: SMEC Closed Loop Scan Test
Test Purpose:	SMEC Close Loop Scan Test.
Initial Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ SMEC ON (close loop)
Final Configuration:	DRCU_ON + AC/DC thermometry ON+MCU ON+ SMEC ON (close loop)
Success Criteria:	Test passed if: SMECENCPOS HK parameter shows identical values as those of the SMECTRAJPOSN HK parameter during the scan.

Test Procedure:

Step#	Action
1	On QLA bring up a time series display of the following SMEC nominal science parameters: SMECENC SIG1 SMECENC SIG2 SMECLVDTDCSIG SMECLVDTAC SIG SMECMOTORCURR
2	Run FUNC-SMEC-07 test procedure from the CCS
3	Contingency: If test fails repeat steps 1.

Test Log:

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	No. of frames received	Test Result
FUNC-SMEC-07	All above mentioned in step 1	N/A	N/A	N/A	Success



First run SMEC_INIT:

Start time:

OBSID: 0xb00002e2

CUS Input Default Parameters:

```
string smec_temp = "warm"; // (cold/warm) Used to specify the PID values
```

Comments: SMECLOOPMODE should change from 6 to 1.

SMEC_07:


Start time: 16:42

OBSID: 0xb00002e3

CUS Input Default Parameters:

```
string smec_temp = "warm"; // (cold/warm) Used to specify the encoder power level  
int scan_start = 1000 in [0,39900]; //Scan starting point (um)  
int scan_end = 15000 in [0,39900]; //Scan ending point (um)  
int scan_fspeed = 200 in [0,2000]; //Scan forward speed (um/s)  
int scan_rspeed = 200 in [0,2000]; //Scan reverse speed (um/s)  
int nscans = 2 in [2,65535]; //Number of scans (has to be even)  
double framerate = 64.0; // Specifies the frame rate
```

Comments: The SMEC remained in closed loop. The encoder signal amplitudes ~2000.

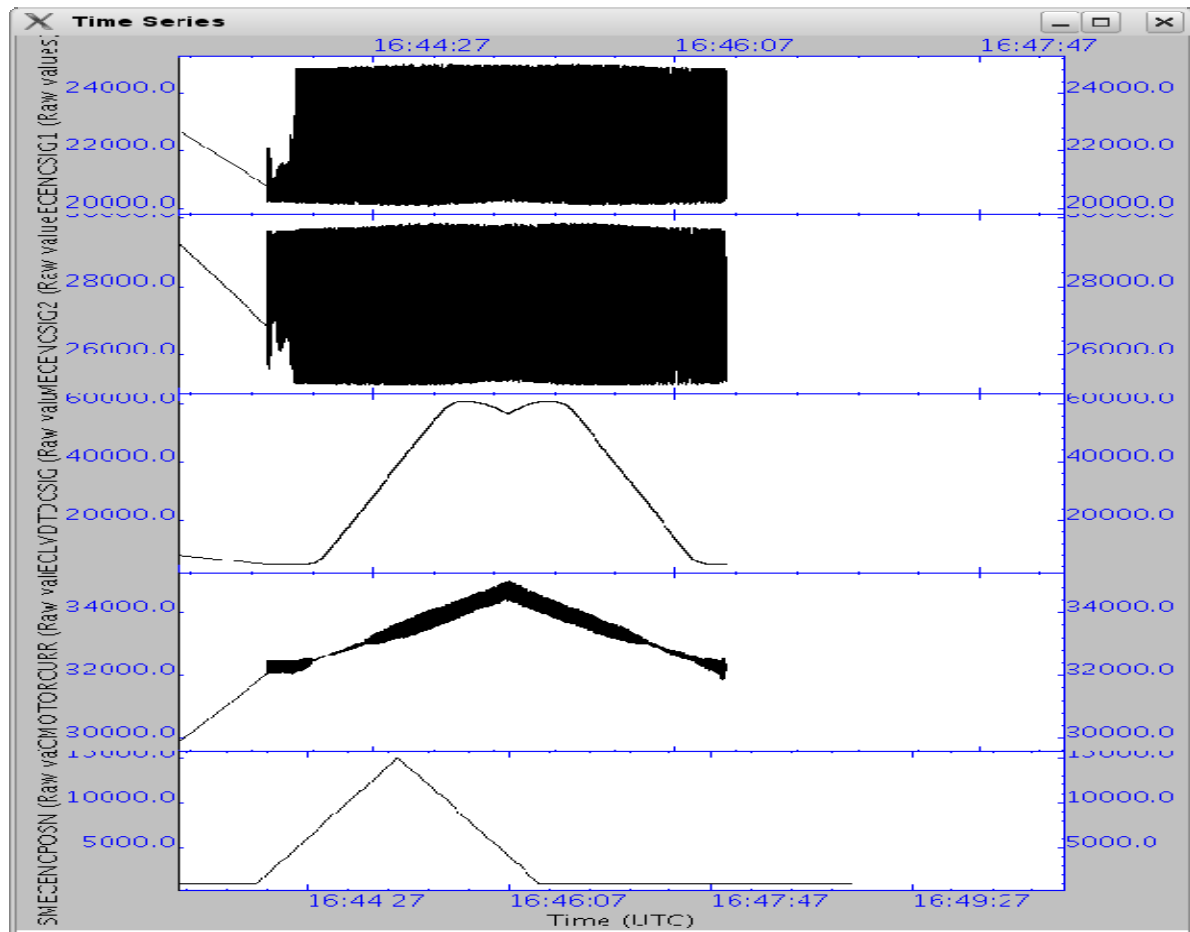



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 86 of 105

4.37 FUNC-SMEC-02B: SMEC Close Launch Latch

Test Id:	FUNC-SMEC-02B: SMEC Close Launch Latch
Initial Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + SMEC ON SMEC Unlatched
Final Configuration:	DRCU_ON + AC/DC thermometry ON +MCU ON + SMEC ON SMEC Latched
Success Criteria:	Test passed if : Prior to un-latching the resistance across pins 7 and 8 of the launch latch is ~ 368 Ohms. After un-latching the resistance is 483 Ohms. Note: These resistance values were recorded for the CQM SMEC model, for the flight SMEC, these values are expected to vary.

Step#	Action	Comments
1	Measure the resistance across pins 7 and 8 of the launch latch.	This step is not applicable anymore
2	Run FUNC-SMEC-02B test procedure from the CCS	
3	Measure the resistance across pins 7 and 8 of the launch latch.	
4	Contingency: If test fails repeat steps 1.	

Test Id	Key Parameter(s)	Expected Value Before/After	Actual Value Before/After	Nb. of frames received	Test Result
FUNC-SMEC-02B				N/A	



Start time: 16:51
OBSID: 0xb00002e4


CUS Input Default Parameters:
string litch = "latch"; // Command SMEC to unlatch

Comments:
After engaging the SMEC latch an attempt is made to perform SMEC scans to see if the SMEC is truly latched.

16:57 Change the FF offset to 0x7000 manually 0x90557000

SMEC-04A:
OBSID: 0xb00002e5

The SMEC moved!!!!!!

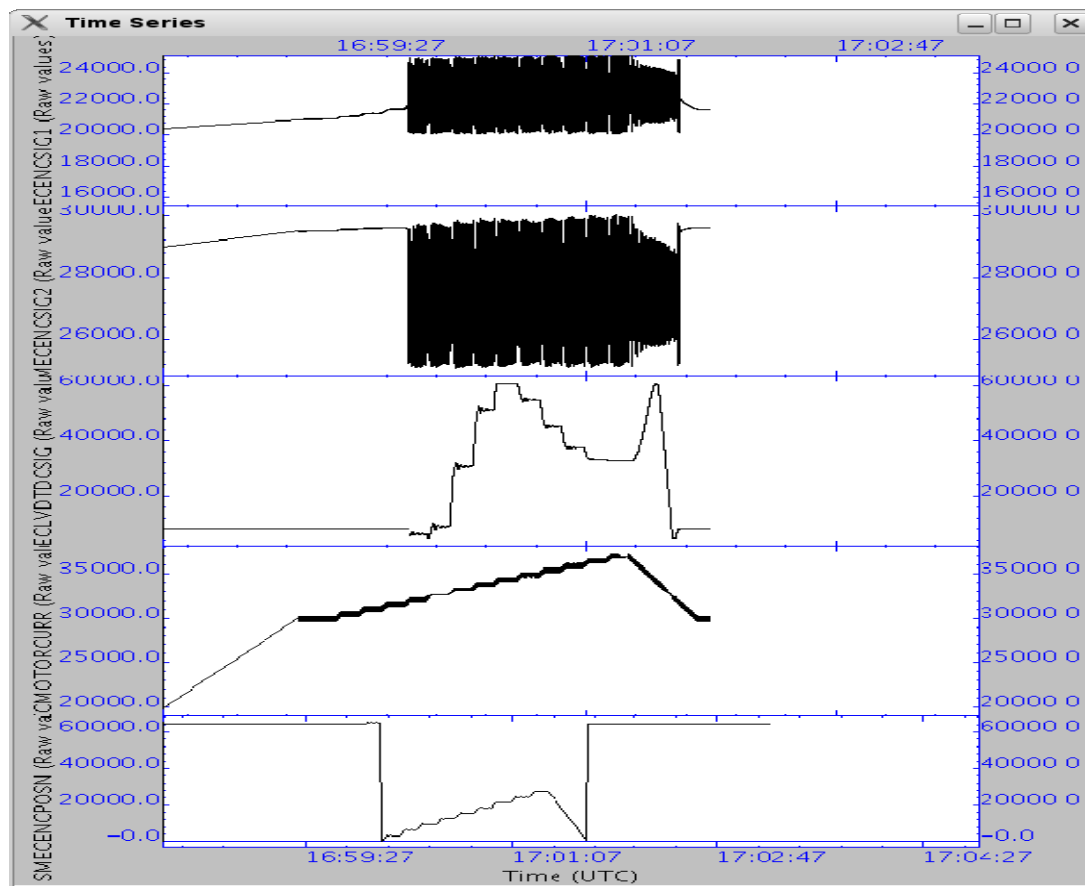

It is not latched

17:07 Set the FF offset to 0 manually 0x90550000
Latch the SMEC manually 0x90430001
Set the FF offset to 0x7000 0x90557000

SMEC-04A:
OBSID: 0xb00002e6
Start time: 17:08


Now the SMEC appears to be latched (Confirmed by Dominique Pouliquen after test).



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 88 of 105

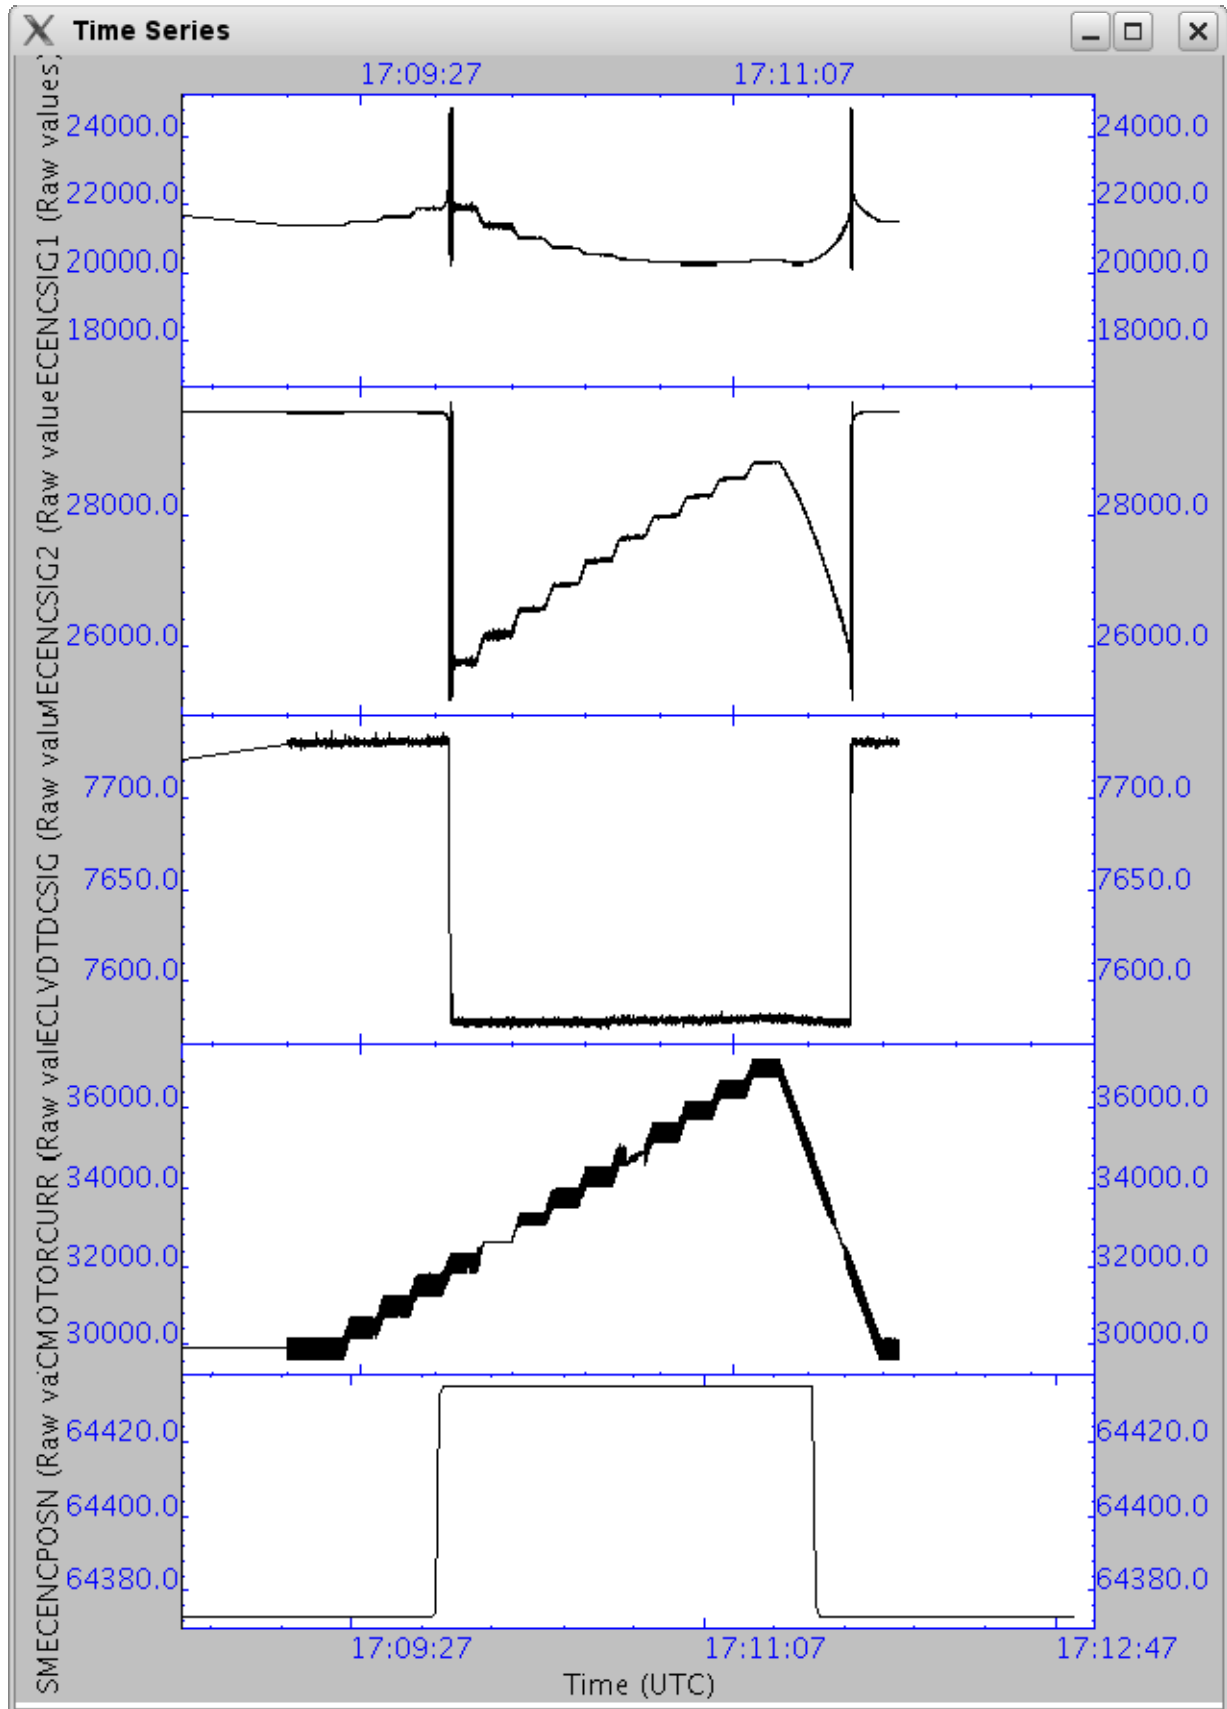



SPIRE Document

**IST WARM FUNCTIONAL TEST REPORT II –
Prime Side
S.D.Sidher & K.J.King**

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	89 of 105

SMEC_OFF:
OBSID: 0xb00002e7
Start time: 17:15

MCU_OFF:
OBSID: 0xb00002e8
Start time: 17:17

SCU_OFF:
OBSID: 0xb00002e9
Start time: 17:19

DRCU_OFF & DPU_OFF



5. ANNEXE 1 (DCU TEST PATTERN DATA)

DCU Photometer Full Array Test Pattern

DCU Test Pattern @ Tue Oct 23 11:15:32 UTC 2007 ..compared with data from DCU Test Pattern @ Wed Mar 14 16:40:00 GMT 2007, OBSID=0x300125CC

Table with 6 columns: Name, New Value[0], New Value[20], Comp Value[0], (Status), Comp Value[20]. Rows list photometer test patterns from PHOTFTSTOBSID to PHOTFTST068.



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	91 of 105

PHOTFTST069	61109.0	61109.0	61109.0	--> OK	61109.0	--> OK
PHOTFTST070	19438.0	19438.0	19438.0	--> OK	19438.0	--> OK
PHOTFTST071	23583.0	23583.0	23583.0	--> OK	23583.0	--> OK
PHOTFTST072	37954.0	37954.0	37954.0	--> OK	37954.0	--> OK
PHOTFTST073	60837.0	60837.0	60837.0	--> OK	60837.0	--> OK
PHOTFTST074	62495.0	62495.0	62495.0	--> OK	62495.0	--> OK
PHOTFTST075	11713.0	11713.0	11713.0	--> OK	11713.0	--> OK
PHOTFTST076	8569.0	8569.0	8569.0	--> OK	8569.0	--> OK
PHOTFTST077	8988.0	8988.0	8988.0	--> OK	8988.0	--> OK
PHOTFTST078	56539.0	56539.0	56539.0	--> OK	56539.0	--> OK
PHOTFTST079	55979.0	55979.0	55979.0	--> OK	55979.0	--> OK
PHOTFTST080	49916.0	49916.0	49916.0	--> OK	49916.0	--> OK
PHOTFTST081	26072.0	26072.0	26072.0	--> OK	26072.0	--> OK
PHOTFTST082	14603.0	14603.0	14603.0	--> OK	14603.0	--> OK
PHOTFTST083	648.0	648.0	648.0	--> OK	648.0	--> OK
PHOTFTST084	49411.0	49411.0	49411.0	--> OK	49411.0	--> OK
PHOTFTST085	27115.0	27115.0	27115.0	--> OK	27115.0	--> OK
PHOTFTST086	62285.0	62285.0	62285.0	--> OK	62285.0	--> OK
PHOTFTST087	1475.0	1475.0	1475.0	--> OK	1475.0	--> OK
PHOTFTST088	26739.0	26739.0	26739.0	--> OK	26739.0	--> OK
PHOTFTST089	17700.0	17700.0	17700.0	--> OK	17700.0	--> OK
PHOTFTST090	7670.0	7670.0	7670.0	--> OK	7670.0	--> OK
PHOTFTST091	45570.0	45570.0	45570.0	--> OK	45570.0	--> OK
PHOTFTST092	36446.0	36446.0	36446.0	--> OK	36446.0	--> OK
PHOTFTST093	32851.0	32851.0	32851.0	--> OK	32851.0	--> OK
PHOTFTST094	76.0	76.0	76.0	--> OK	76.0	--> OK
PHOTFTST095	59353.0	59353.0	59353.0	--> OK	59353.0	--> OK
PHOTFTST096	14681.0	14681.0	14681.0	--> OK	14681.0	--> OK
PHOTFTST097	45993.0	45993.0	45993.0	--> OK	45993.0	--> OK
PHOTFTST098	3039.0	3039.0	3039.0	--> OK	3039.0	--> OK
PHOTFTST099	21485.0	21485.0	21485.0	--> OK	21485.0	--> OK
PHOTFTST100	58423.0	58423.0	58423.0	--> OK	58423.0	--> OK
PHOTFTST101	49530.0	49530.0	49530.0	--> OK	49530.0	--> OK
PHOTFTST102	59672.0	59672.0	59672.0	--> OK	59672.0	--> OK
PHOTFTST103	39150.0	39150.0	39150.0	--> OK	39150.0	--> OK
PHOTFTST104	61616.0	61616.0	61616.0	--> OK	61616.0	--> OK
PHOTFTST105	6295.0	6295.0	6295.0	--> OK	6295.0	--> OK
PHOTFTST106	30262.0	30262.0	30262.0	--> OK	30262.0	--> OK
PHOTFTST107	20736.0	20736.0	20736.0	--> OK	20736.0	--> OK
PHOTFTST108	15460.0	15460.0	15460.0	--> OK	15460.0	--> OK
PHOTFTST109	62270.0	62270.0	62270.0	--> OK	62270.0	--> OK
PHOTFTST110	42095.0	42095.0	42095.0	--> OK	42095.0	--> OK
PHOTFTST111	43075.0	43075.0	43075.0	--> OK	43075.0	--> OK
PHOTFTST112	61472.0	61472.0	61472.0	--> OK	61472.0	--> OK
PHOTFTST113	25519.0	25519.0	25519.0	--> OK	25519.0	--> OK
PHOTFTST114	423.0	423.0	423.0	--> OK	423.0	--> OK
PHOTFTST115	13689.0	13689.0	13689.0	--> OK	13689.0	--> OK
PHOTFTST116	57692.0	57692.0	57692.0	--> OK	57692.0	--> OK
PHOTFTST117	35227.0	35227.0	35227.0	--> OK	35227.0	--> OK
PHOTFTST118	40405.0	40405.0	40405.0	--> OK	40405.0	--> OK
PHOTFTST119	33222.0	33222.0	33222.0	--> OK	33222.0	--> OK
PHOTFTST120	25871.0	25871.0	25871.0	--> OK	25871.0	--> OK
PHOTFTST121	35174.0	35174.0	35174.0	--> OK	35174.0	--> OK
PHOTFTST122	49587.0	49587.0	49587.0	--> OK	49587.0	--> OK
PHOTFTST123	60595.0	60595.0	60595.0	--> OK	60595.0	--> OK
PHOTFTST124	58121.0	58121.0	58121.0	--> OK	58121.0	--> OK
PHOTFTST125	39089.0	39089.0	39089.0	--> OK	39089.0	--> OK
PHOTFTST126	40086.0	40086.0	40086.0	--> OK	40086.0	--> OK
PHOTFTST127	61336.0	61336.0	61336.0	--> OK	61336.0	--> OK
PHOTFTST128	36067.0	36067.0	36067.0	--> OK	36067.0	--> OK
PHOTFTST129	15197.0	15197.0	15197.0	--> OK	15197.0	--> OK
PHOTFTST130	54572.0	54572.0	54572.0	--> OK	54572.0	--> OK
PHOTFTST131	3320.0	3320.0	3320.0	--> OK	3320.0	--> OK
PHOTFTST132	23946.0	23946.0	23946.0	--> OK	23946.0	--> OK
PHOTFTST133	62588.0	62588.0	62588.0	--> OK	62588.0	--> OK
PHOTFTST134	33562.0	33562.0	33562.0	--> OK	33562.0	--> OK
PHOTFTST135	58279.0	58279.0	58279.0	--> OK	58279.0	--> OK
PHOTFTST136	63609.0	63609.0	63609.0	--> OK	63609.0	--> OK
PHOTFTST137	13326.0	13326.0	13326.0	--> OK	13326.0	--> OK
PHOTFTST138	31406.0	31406.0	31406.0	--> OK	31406.0	--> OK
PHOTFTST139	30437.0	30437.0	30437.0	--> OK	30437.0	--> OK
PHOTFTST140	50814.0	50814.0	50814.0	--> OK	50814.0	--> OK
PHOTFTST141	61182.0	61182.0	61182.0	--> OK	61182.0	--> OK
PHOTFTST142	16832.0	16832.0	16832.0	--> OK	16832.0	--> OK
PHOTFTST143	47199.0	47199.0	47199.0	--> OK	47199.0	--> OK
PHOTFTST144	269.0	269.0	269.0	--> OK	269.0	--> OK
PHOTFTST145	4261.0	4261.0	4261.0	--> OK	4261.0	--> OK
PHOTFTST146	62990.0	62990.0	62990.0	--> OK	62990.0	--> OK
PHOTFTST147	43420.0	43420.0	43420.0	--> OK	43420.0	--> OK
PHOTFTST148	14880.0	14880.0	14880.0	--> OK	14880.0	--> OK
PHOTFTST149	50504.0	50504.0	50504.0	--> OK	50504.0	--> OK
PHOTFTST150	22549.0	22549.0	22549.0	--> OK	22549.0	--> OK
PHOTFTST151	44210.0	44210.0	44210.0	--> OK	44210.0	--> OK
PHOTFTST152	64905.0	64905.0	64905.0	--> OK	64905.0	--> OK
PHOTFTST153	61431.0	61431.0	61431.0	--> OK	61431.0	--> OK
PHOTFTST154	62465.0	62465.0	62465.0	--> OK	62465.0	--> OK



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	92 of 105

PHOTFTST155	61851.0	61851.0	61851.0	--> OK	61851.0	--> OK
PHOTFTST156	39333.0	39333.0	39333.0	--> OK	39333.0	--> OK
PHOTFTST157	45823.0	45823.0	45823.0	--> OK	45823.0	--> OK
PHOTFTST158	53816.0	53816.0	53816.0	--> OK	53816.0	--> OK
PHOTFTST159	60710.0	60710.0	60710.0	--> OK	60710.0	--> OK
PHOTFTST160	34378.0	34378.0	34378.0	--> OK	34378.0	--> OK
PHOTFTST161	25724.0	25724.0	25724.0	--> OK	25724.0	--> OK
PHOTFTST162	60897.0	60897.0	60897.0	--> OK	60897.0	--> OK
PHOTFTST163	12140.0	12140.0	12140.0	--> OK	12140.0	--> OK
PHOTFTST164	14299.0	14299.0	14299.0	--> OK	14299.0	--> OK
PHOTFTST165	6883.0	6883.0	6883.0	--> OK	6883.0	--> OK
PHOTFTST166	20030.0	20030.0	20030.0	--> OK	20030.0	--> OK
PHOTFTST167	4598.0	4598.0	4598.0	--> OK	4598.0	--> OK
PHOTFTST168	7984.0	7984.0	7984.0	--> OK	7984.0	--> OK
PHOTFTST169	17054.0	17054.0	17054.0	--> OK	17054.0	--> OK
PHOTFTST170	22076.0	22076.0	22076.0	--> OK	22076.0	--> OK
PHOTFTST171	49498.0	49498.0	49498.0	--> OK	49498.0	--> OK
PHOTFTST172	3680.0	3680.0	3680.0	--> OK	3680.0	--> OK
PHOTFTST173	40243.0	40243.0	40243.0	--> OK	40243.0	--> OK
PHOTFTST174	40825.0	40825.0	40825.0	--> OK	40825.0	--> OK
PHOTFTST175	58735.0	58735.0	58735.0	--> OK	58735.0	--> OK
PHOTFTST176	6296.0	6296.0	6296.0	--> OK	6296.0	--> OK
PHOTFTST177	44890.0	44890.0	44890.0	--> OK	44890.0	--> OK
PHOTFTST178	11975.0	11975.0	11975.0	--> OK	11975.0	--> OK
PHOTFTST179	42645.0	42645.0	42645.0	--> OK	42645.0	--> OK
PHOTFTST180	51549.0	51549.0	51549.0	--> OK	51549.0	--> OK
PHOTFTST181	7571.0	7571.0	7571.0	--> OK	7571.0	--> OK
PHOTFTST182	14165.0	14165.0	14165.0	--> OK	14165.0	--> OK
PHOTFTST183	54769.0	54769.0	54769.0	--> OK	54769.0	--> OK
PHOTFTST184	58235.0	58235.0	58235.0	--> OK	58235.0	--> OK
PHOTFTST185	13602.0	13602.0	13602.0	--> OK	13602.0	--> OK
PHOTFTST186	6350.0	6350.0	6350.0	--> OK	6350.0	--> OK
PHOTFTST187	28469.0	28469.0	28469.0	--> OK	28469.0	--> OK
PHOTFTST188	16254.0	16254.0	16254.0	--> OK	16254.0	--> OK
PHOTFTST189	18355.0	18355.0	18355.0	--> OK	18355.0	--> OK
PHOTFTST190	32290.0	32290.0	32290.0	--> OK	32290.0	--> OK
PHOTFTST191	10077.0	10077.0	10077.0	--> OK	10077.0	--> OK
PHOTFTST192	22612.0	22612.0	22612.0	--> OK	22612.0	--> OK
PHOTFTST193	62886.0	62886.0	62886.0	--> OK	62886.0	--> OK
PHOTFTST194	31171.0	31171.0	31171.0	--> OK	31171.0	--> OK
PHOTFTST195	30969.0	30969.0	30969.0	--> OK	30969.0	--> OK
PHOTFTST196	52642.0	52642.0	52642.0	--> OK	52642.0	--> OK
PHOTFTST197	20461.0	20461.0	20461.0	--> OK	20461.0	--> OK
PHOTFTST198	26959.0	26959.0	26959.0	--> OK	26959.0	--> OK
PHOTFTST199	58181.0	58181.0	58181.0	--> OK	58181.0	--> OK
PHOTFTST200	1736.0	1736.0	1736.0	--> OK	1736.0	--> OK
PHOTFTST201	42447.0	42447.0	42447.0	--> OK	42447.0	--> OK
PHOTFTST202	55791.0	55791.0	55791.0	--> OK	55791.0	--> OK
PHOTFTST203	52325.0	52325.0	52325.0	--> OK	52325.0	--> OK
PHOTFTST204	16702.0	16702.0	16702.0	--> OK	16702.0	--> OK
PHOTFTST205	34421.0	34421.0	34421.0	--> OK	34421.0	--> OK
PHOTFTST206	41152.0	41152.0	41152.0	--> OK	41152.0	--> OK
PHOTFTST207	40213.0	40213.0	40213.0	--> OK	40213.0	--> OK
PHOTFTST208	42863.0	42863.0	42863.0	--> OK	42863.0	--> OK
PHOTFTST209	33552.0	33552.0	33552.0	--> OK	33552.0	--> OK
PHOTFTST210	27975.0	27975.0	27975.0	--> OK	27975.0	--> OK
PHOTFTST211	21482.0	21482.0	21482.0	--> OK	21482.0	--> OK
PHOTFTST212	40500.0	40500.0	40500.0	--> OK	40500.0	--> OK
PHOTFTST213	7267.0	7267.0	7267.0	--> OK	7267.0	--> OK
PHOTFTST214	19270.0	19270.0	19270.0	--> OK	19270.0	--> OK
PHOTFTST215	57569.0	57569.0	57569.0	--> OK	57569.0	--> OK
PHOTFTST216	42411.0	42411.0	42411.0	--> OK	42411.0	--> OK
PHOTFTST217	54772.0	54772.0	54772.0	--> OK	54772.0	--> OK
PHOTFTST218	54178.0	54178.0	54178.0	--> OK	54178.0	--> OK
PHOTFTST219	24811.0	24811.0	24811.0	--> OK	24811.0	--> OK
PHOTFTST220	5807.0	5807.0	5807.0	--> OK	5807.0	--> OK
PHOTFTST221	23635.0	23635.0	23635.0	--> OK	23635.0	--> OK
PHOTFTST222	58479.0	58479.0	58479.0	--> OK	58479.0	--> OK
PHOTFTST223	54524.0	54524.0	54524.0	--> OK	54524.0	--> OK
PHOTFTST224	49934.0	49934.0	49934.0	--> OK	49934.0	--> OK
PHOTFTST225	55320.0	55320.0	55320.0	--> OK	55320.0	--> OK
PHOTFTST226	54244.0	54244.0	54244.0	--> OK	54244.0	--> OK
PHOTFTST227	43319.0	43319.0	43319.0	--> OK	43319.0	--> OK
PHOTFTST228	33893.0	33893.0	33893.0	--> OK	33893.0	--> OK
PHOTFTST229	14361.0	14361.0	14361.0	--> OK	14361.0	--> OK
PHOTFTST230	49700.0	49700.0	49700.0	--> OK	49700.0	--> OK
PHOTFTST231	26066.0	26066.0	26066.0	--> OK	26066.0	--> OK
PHOTFTST232	22713.0	22713.0	22713.0	--> OK	22713.0	--> OK
PHOTFTST233	43291.0	43291.0	43291.0	--> OK	43291.0	--> OK
PHOTFTST234	56769.0	56769.0	56769.0	--> OK	56769.0	--> OK
PHOTFTST235	3878.0	3878.0	3878.0	--> OK	3878.0	--> OK
PHOTFTST236	17774.0	17774.0	17774.0	--> OK	17774.0	--> OK
PHOTFTST237	9052.0	9052.0	9052.0	--> OK	9052.0	--> OK
PHOTFTST238	4650.0	4650.0	4650.0	--> OK	4650.0	--> OK
PHOTFTST239	53520.0	53520.0	53520.0	--> OK	53520.0	--> OK
PHOTFTST240	7534.0	7534.0	7534.0	--> OK	7534.0	--> OK



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	93 of 105

PHOTFTST241	39702.0	39702.0	39702.0	--> OK	39702.0	--> OK
PHOTFTST242	53314.0	53314.0	53314.0	--> OK	53314.0	--> OK
PHOTFTST243	21275.0	21275.0	21275.0	--> OK	21275.0	--> OK
PHOTFTST244	31886.0	31886.0	31886.0	--> OK	31886.0	--> OK
PHOTFTST245	17396.0	17396.0	17396.0	--> OK	17396.0	--> OK
PHOTFTST246	9667.0	9667.0	9667.0	--> OK	9667.0	--> OK
PHOTFTST247	19008.0	19008.0	19008.0	--> OK	19008.0	--> OK
PHOTFTST248	56499.0	56499.0	56499.0	--> OK	56499.0	--> OK
PHOTFTST249	4661.0	4661.0	4661.0	--> OK	4661.0	--> OK
PHOTFTST250	61401.0	61401.0	61401.0	--> OK	61401.0	--> OK
PHOTFTST251	57818.0	57818.0	57818.0	--> OK	57818.0	--> OK
PHOTFTST252	20084.0	20084.0	20084.0	--> OK	20084.0	--> OK
PHOTFTST253	5075.0	5075.0	5075.0	--> OK	5075.0	--> OK
PHOTFTST254	48920.0	48920.0	48920.0	--> OK	48920.0	--> OK
PHOTFTST255	20309.0	20309.0	20309.0	--> OK	20309.0	--> OK
PHOTFTST256	51969.0	51969.0	51969.0	--> OK	51969.0	--> OK
PHOTFTST257	20797.0	20797.0	20797.0	--> OK	20797.0	--> OK
PHOTFTST258	13073.0	13073.0	13073.0	--> OK	13073.0	--> OK
PHOTFTST259	33415.0	33415.0	33415.0	--> OK	33415.0	--> OK
PHOTFTST260	17118.0	17118.0	17118.0	--> OK	17118.0	--> OK
PHOTFTST261	46469.0	46469.0	46469.0	--> OK	46469.0	--> OK
PHOTFTST262	51937.0	51937.0	51937.0	--> OK	51937.0	--> OK
PHOTFTST263	33458.0	33458.0	33458.0	--> OK	33458.0	--> OK
PHOTFTST264	26307.0	26307.0	26307.0	--> OK	26307.0	--> OK
PHOTFTST265	59263.0	59263.0	59263.0	--> OK	59263.0	--> OK
PHOTFTST266	40109.0	40109.0	40109.0	--> OK	40109.0	--> OK
PHOTFTST267	45776.0	45776.0	45776.0	--> OK	45776.0	--> OK
PHOTFTST268	25643.0	25643.0	25643.0	--> OK	25643.0	--> OK
PHOTFTST269	5793.0	5793.0	5793.0	--> OK	5793.0	--> OK
PHOTFTST270	64288.0	64288.0	64288.0	--> OK	64288.0	--> OK
PHOTFTST271	24157.0	24157.0	24157.0	--> OK	24157.0	--> OK
PHOTFTST272	26592.0	26592.0	26592.0	--> OK	26592.0	--> OK
PHOTFTST273	31527.0	31527.0	31527.0	--> OK	31527.0	--> OK
PHOTFTST274	54598.0	54598.0	54598.0	--> OK	54598.0	--> OK
PHOTFTST275	39117.0	39117.0	39117.0	--> OK	39117.0	--> OK
PHOTFTST276	63615.0	63615.0	63615.0	--> OK	63615.0	--> OK
PHOTFTST277	53746.0	53746.0	53746.0	--> OK	53746.0	--> OK
PHOTFTST278	58335.0	58335.0	58335.0	--> OK	58335.0	--> OK
PHOTFTST279	16933.0	16933.0	16933.0	--> OK	16933.0	--> OK
PHOTFTST280	7109.0	7109.0	7109.0	--> OK	7109.0	--> OK
PHOTFTST281	16101.0	16101.0	16101.0	--> OK	16101.0	--> OK
PHOTFTST282	41909.0	41909.0	41909.0	--> OK	41909.0	--> OK
PHOTFTST283	43695.0	43695.0	43695.0	--> OK	43695.0	--> OK
PHOTFTST284	36126.0	36126.0	36126.0	--> OK	36126.0	--> OK
PHOTFTST285	32243.0	32243.0	32243.0	--> OK	32243.0	--> OK
PHOTFTST286	30919.0	30919.0	30919.0	--> OK	30919.0	--> OK
PHOTFTST287	28974.0	28974.0	28974.0	--> OK	28974.0	--> OK
PHOTFTST288	62188.0	62188.0	62188.0	--> OK	62188.0	--> OK
PHOTFTSTADCF LGS	0.0	0.0	0.0	--> OK	0.0	--> OK
PHOTFTSTFRAMETIME	8439844.0	8847519.0	1.0253174E7	<--BAD	1.0589166E7	<--BAD
PHOTFTSTCHECKWORD	12473.0	63493.0	35831.0		27474.0	

Note that the frame values indicated “BAD” are actually expected to be different from test to test, i.e. frame time, check word and observation identifier, etc.



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref:	SPIRE-RAL-REP-002991
Issue:	1.1
Date:	19/04/2008
Page:	94 of 105

DCU Spectrometer Full Array Test Pattern

DCU Test Pattern @ Tue Oct 23 11:15:57 UTC 2007

..compared with data from DCU Test Pattern @ Wed Mar 14 16:40:34 GMT 2007, OBSID=0x300125CC

Name	New Value[0]	New Value[20]	Comp Value[0]	Comp Value[20]
SPECFTSTOBSID	0xB00002CF	0x0	0x300125CC	0x0
SPECFTSTBBID	0x88080001	0x0	0x88080001	--> OK 0x0 --> OK
SPECFTSTBLKLEN	78.0	78.0	78.0	--> OK 78.0 --> OK
SPECFTSTFRAMEID	13.0	13.0	13.0	--> OK 13.0 --> OK
SPECFTST001	6583.0	6583.0	6583.0	--> OK 6583.0 --> OK
SPECFTST002	23180.0	23180.0	23180.0	--> OK 23180.0 --> OK
SPECFTST003	31282.0	31282.0	31282.0	--> OK 31282.0 --> OK
SPECFTST004	53988.0	53988.0	53988.0	--> OK 53988.0 --> OK
SPECFTST005	57605.0	57605.0	57605.0	--> OK 57605.0 --> OK
SPECFTST006	43658.0	43658.0	43658.0	--> OK 43658.0 --> OK
SPECFTST007	62379.0	62379.0	62379.0	--> OK 62379.0 --> OK
SPECFTST008	11751.0	11751.0	11751.0	--> OK 11751.0 --> OK
SPECFTST009	59411.0	59411.0	59411.0	--> OK 59411.0 --> OK
SPECFTST010	49072.0	49072.0	49072.0	--> OK 49072.0 --> OK
SPECFTST011	12708.0	12708.0	12708.0	--> OK 12708.0 --> OK
SPECFTST012	64232.0	64232.0	64232.0	--> OK 64232.0 --> OK
SPECFTST013	30471.0	30471.0	30471.0	--> OK 30471.0 --> OK
SPECFTST014	53034.0	53034.0	53034.0	--> OK 53034.0 --> OK
SPECFTST015	20944.0	20944.0	20944.0	--> OK 20944.0 --> OK
SPECFTST016	164.0	164.0	164.0	--> OK 164.0 --> OK
SPECFTST017	60700.0	60700.0	60700.0	--> OK 60700.0 --> OK
SPECFTST018	779.0	779.0	779.0	--> OK 779.0 --> OK
SPECFTST019	23214.0	23214.0	23214.0	--> OK 23214.0 --> OK
SPECFTST020	40139.0	40139.0	40139.0	--> OK 40139.0 --> OK
SPECFTST021	24553.0	24553.0	24553.0	--> OK 24553.0 --> OK
SPECFTST022	62268.0	62268.0	62268.0	--> OK 62268.0 --> OK
SPECFTST023	7195.0	7195.0	7195.0	--> OK 7195.0 --> OK
SPECFTST024	8339.0	8339.0	8339.0	--> OK 8339.0 --> OK
SPECFTST025	45993.0	45993.0	45993.0	--> OK 45993.0 --> OK
SPECFTST026	62270.0	62270.0	62270.0	--> OK 62270.0 --> OK
SPECFTST027	21485.0	21485.0	21485.0	--> OK 21485.0 --> OK
SPECFTST028	43075.0	43075.0	43075.0	--> OK 43075.0 --> OK
SPECFTST029	49530.0	49530.0	49530.0	--> OK 49530.0 --> OK
SPECFTST030	3039.0	3039.0	3039.0	--> OK 3039.0 --> OK
SPECFTST031	39150.0	39150.0	39150.0	--> OK 39150.0 --> OK
SPECFTST032	58423.0	58423.0	58423.0	--> OK 58423.0 --> OK
SPECFTST033	6295.0	6295.0	6295.0	--> OK 6295.0 --> OK
SPECFTST034	59672.0	59672.0	59672.0	--> OK 59672.0 --> OK
SPECFTST035	20736.0	20736.0	20736.0	--> OK 20736.0 --> OK
SPECFTST036	61616.0	61616.0	61616.0	--> OK 61616.0 --> OK
SPECFTST037	4261.0	4261.0	4261.0	--> OK 4261.0 --> OK
SPECFTST038	45823.0	45823.0	45823.0	--> OK 45823.0 --> OK
SPECFTST039	43420.0	43420.0	43420.0	--> OK 43420.0 --> OK
SPECFTST040	60710.0	60710.0	60710.0	--> OK 60710.0 --> OK
SPECFTST041	50504.0	50504.0	50504.0	--> OK 50504.0 --> OK
SPECFTST042	62990.0	62990.0	62990.0	--> OK 62990.0 --> OK
SPECFTST043	44210.0	44210.0	44210.0	--> OK 44210.0 --> OK
SPECFTST044	14880.0	14880.0	14880.0	--> OK 14880.0 --> OK
SPECFTST045	61431.0	61431.0	61431.0	--> OK 61431.0 --> OK
SPECFTST046	22549.0	22549.0	22549.0	--> OK 22549.0 --> OK
SPECFTST047	61851.0	61851.0	61851.0	--> OK 61851.0 --> OK
SPECFTST048	64905.0	64905.0	64905.0	--> OK 64905.0 --> OK
SPECFTST049	62886.0	62886.0	62886.0	--> OK 62886.0 --> OK
SPECFTST050	34421.0	34421.0	34421.0	--> OK 34421.0 --> OK
SPECFTST051	30969.0	30969.0	30969.0	--> OK 30969.0 --> OK
SPECFTST052	40213.0	40213.0	40213.0	--> OK 40213.0 --> OK
SPECFTST053	20461.0	20461.0	20461.0	--> OK 20461.0 --> OK
SPECFTST054	31171.0	31171.0	31171.0	--> OK 31171.0 --> OK
SPECFTST055	58181.0	58181.0	58181.0	--> OK 58181.0 --> OK
SPECFTST056	52642.0	52642.0	52642.0	--> OK 52642.0 --> OK
SPECFTST057	42447.0	42447.0	42447.0	--> OK 42447.0 --> OK
SPECFTST058	26959.0	26959.0	26959.0	--> OK 26959.0 --> OK
SPECFTST059	52325.0	52325.0	52325.0	--> OK 52325.0 --> OK
SPECFTST060	1736.0	1736.0	1736.0	--> OK 1736.0 --> OK
SPECFTST061	39702.0	39702.0	39702.0	--> OK 39702.0 --> OK
SPECFTST062	5075.0	5075.0	5075.0	--> OK 5075.0 --> OK
SPECFTST063	21275.0	21275.0	21275.0	--> OK 21275.0 --> OK
SPECFTST064	20309.0	20309.0	20309.0	--> OK 20309.0 --> OK
SPECFTST065	17396.0	17396.0	17396.0	--> OK 17396.0 --> OK
SPECFTST066	53314.0	53314.0	53314.0	--> OK 53314.0 --> OK
SPECFTST067	19008.0	19008.0	19008.0	--> OK 19008.0 --> OK
SPECFTST068	31886.0	31886.0	31886.0	--> OK 31886.0 --> OK



SPIRE Document

IST WARM FUNCTIONAL TEST REPORT II – Prime Side S.D.Sidher & K.J.King

Ref: SPIRE-RAL-REP-002991
Issue: 1.1
Date: 19/04/2008
Page: 95 of 105

SPECFTST069	4661.0	4661.0	4661.0	--> OK	4661.0	--> OK
SPECFTST070	9667.0	9667.0	9667.0	--> OK	9667.0	--> OK
SPECFTST071	57818.0	57818.0	57818.0	--> OK	57818.0	--> OK
SPECFTST072	56499.0	56499.0	56499.0	--> OK	56499.0	--> OK
SPECFTSTADCFGLS	0.0	0.0	0.0	--> OK	0.0	--> OK
SPECFTSTFRAMETIME	1.7812933E7	1.7891012E7	2.2126281E7		2.2204359E7	
SPECFTSTCHECKWORD	26935.0	23081.0	14949.0		27496.0	

6. ANNEXE 2 (RESULTS OF LOAD CURVES)

The following graphs (1-12) show the response of the 288 Photometer detectors to the input voltage during the Load Curve (FUNC-DCU-13). The graph (13) shows the response of the 3 PTC channels to the input voltage during the Load Curve. The graphs (14-16) show the spectrometer 78 detectors output voltage during the load curve performed on the spectrometer side. These plots are for OBSIDS B0000217 for photometer and B000021C for spectrometer. For all the photometer load curves the first anomalous point has been removed from the plots.

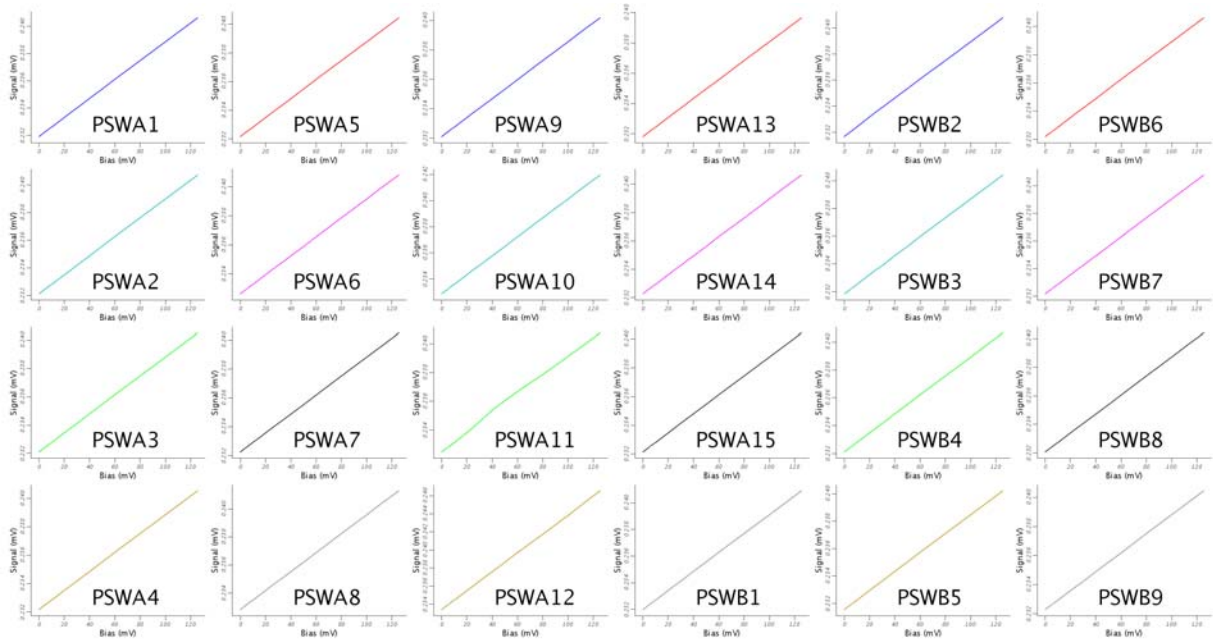


Figure 1. PSW Detectors (1)

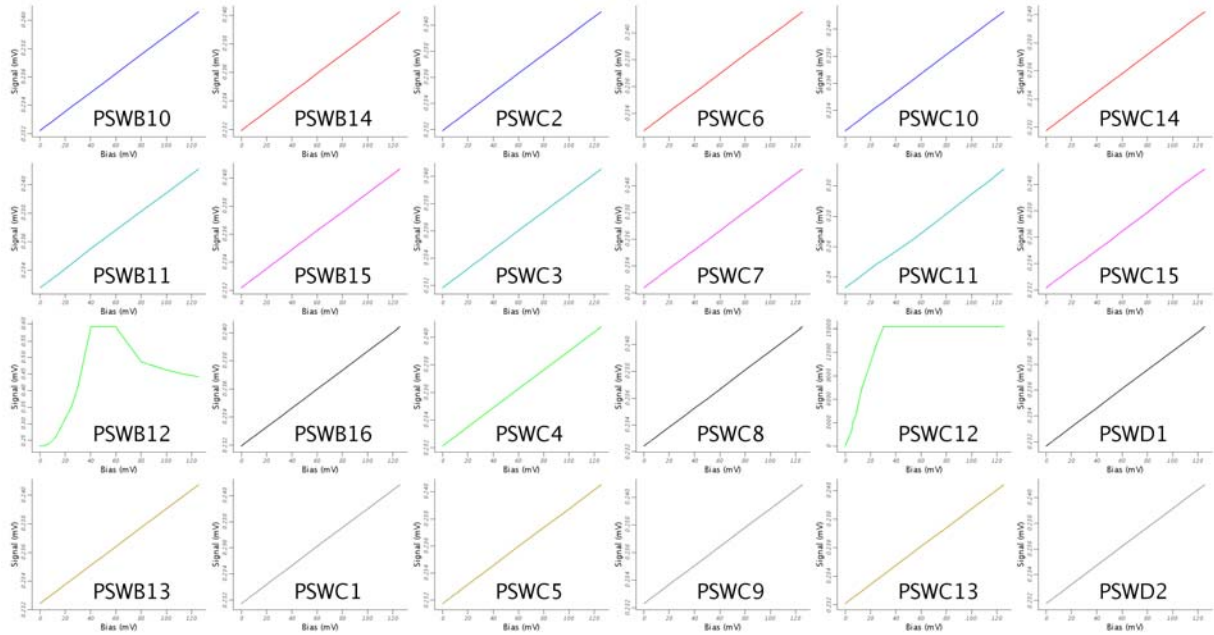


Figure 2. PSW Detectors (2)

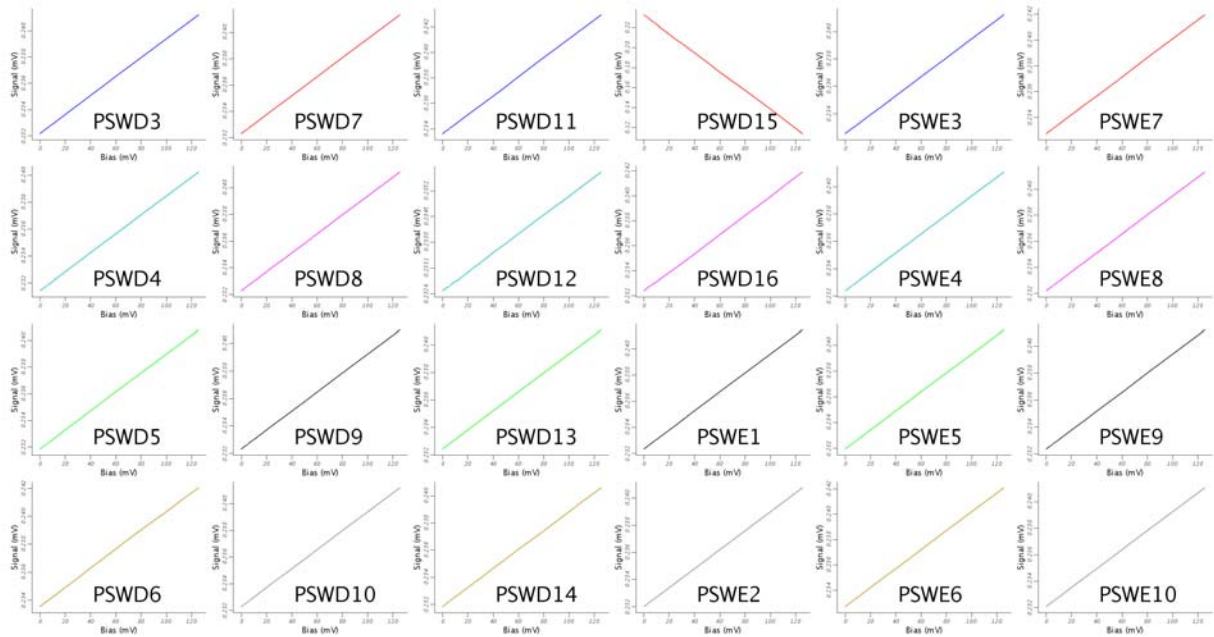


Figure 3. PSW Detectors (3)

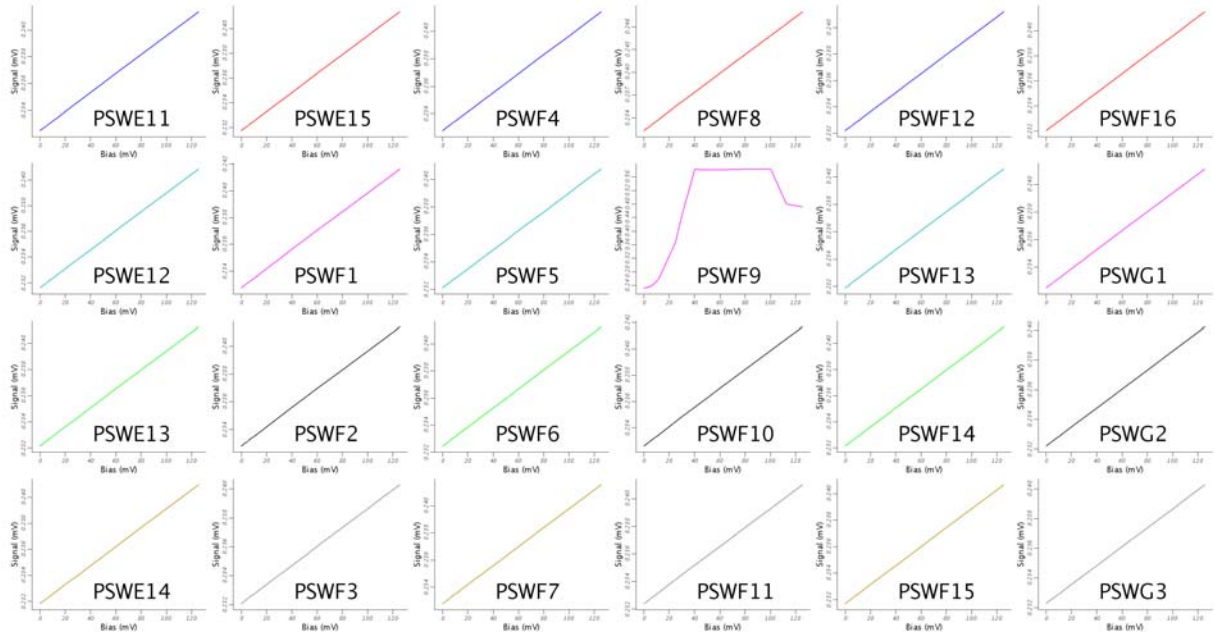


Figure 4. PSW Detectors (4)

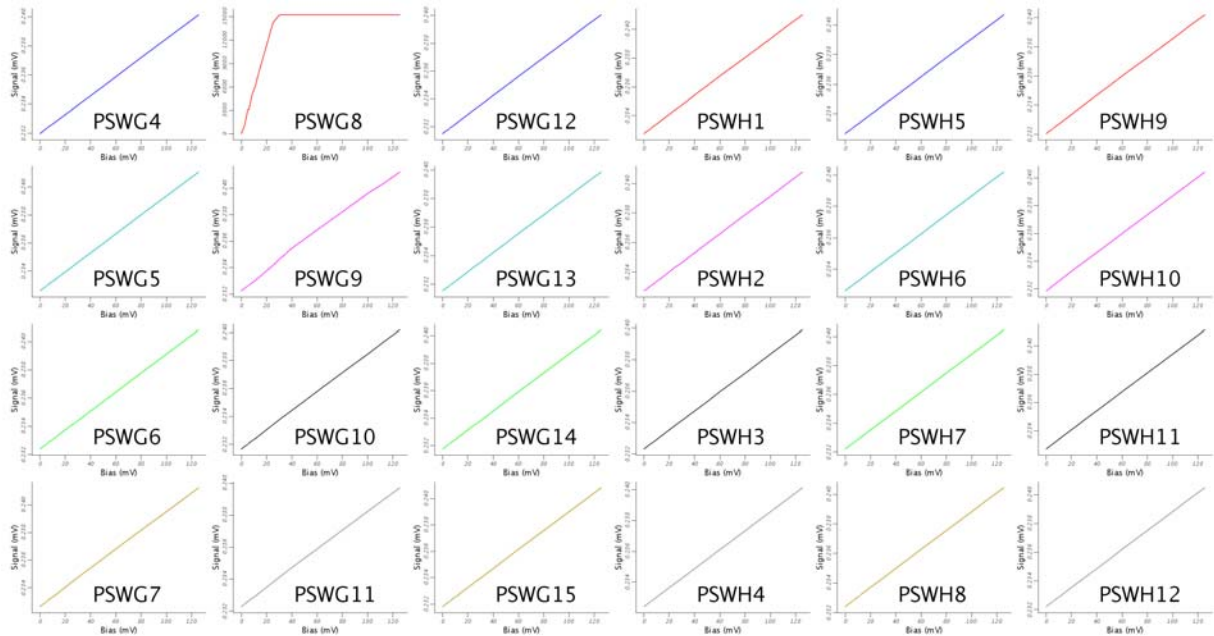


Figure 5. PSW Detectors (5)

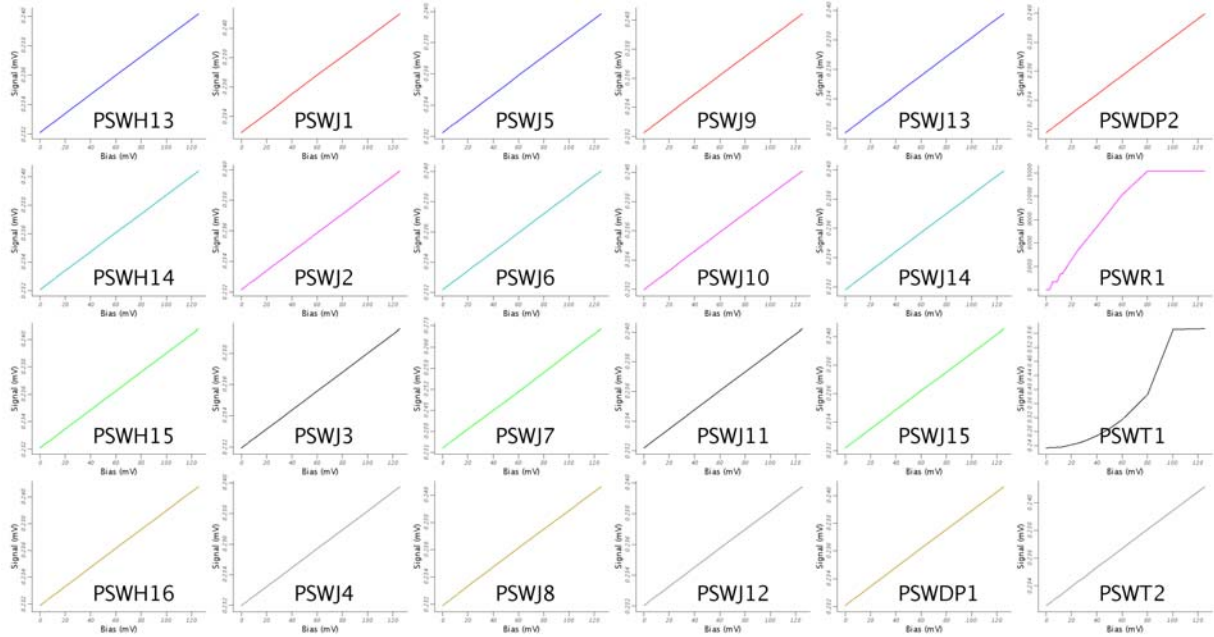


Figure 6. PSW Detectors (6)

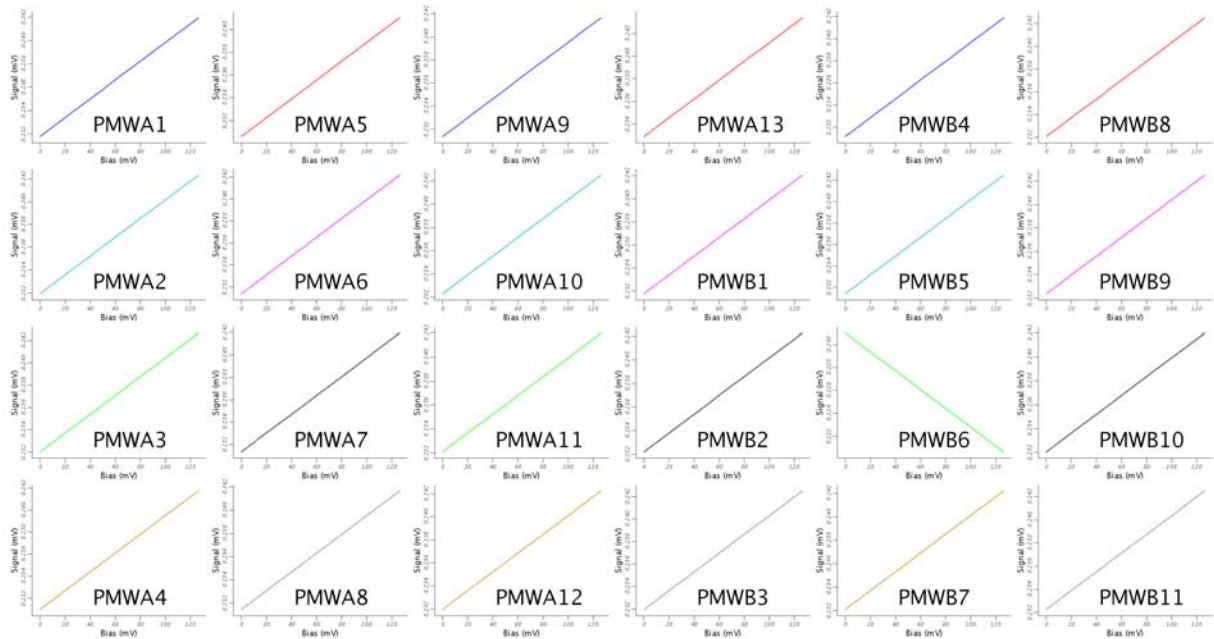


Figure 7. PMW Detectors (1)

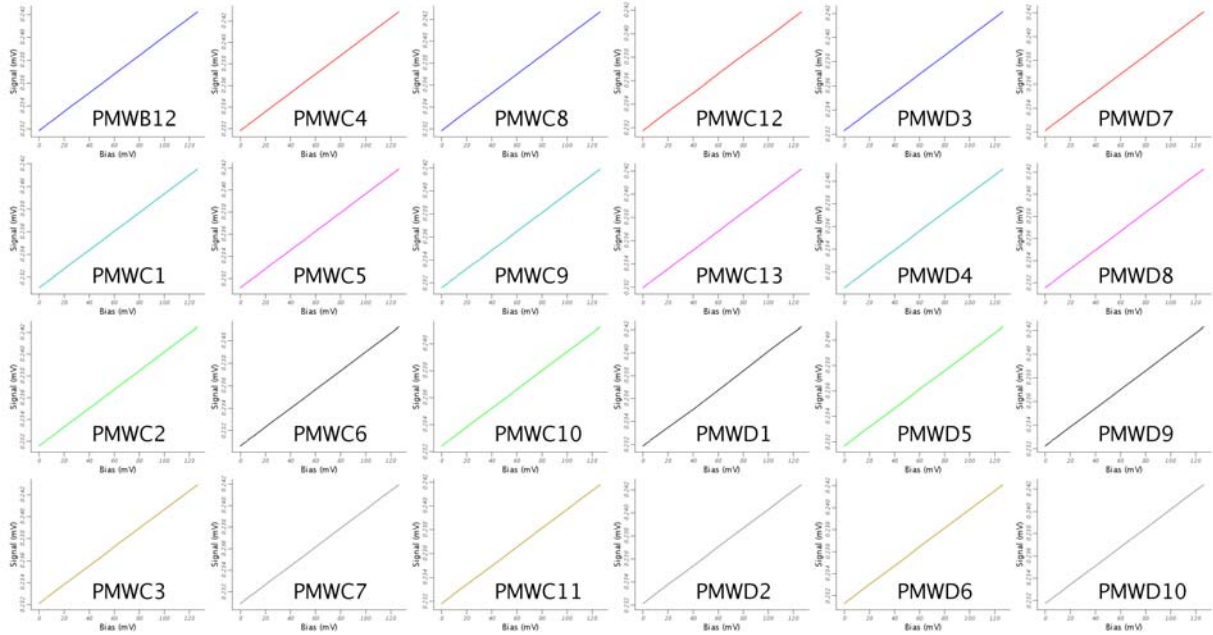


Figure 8. PMW Detectors (2)

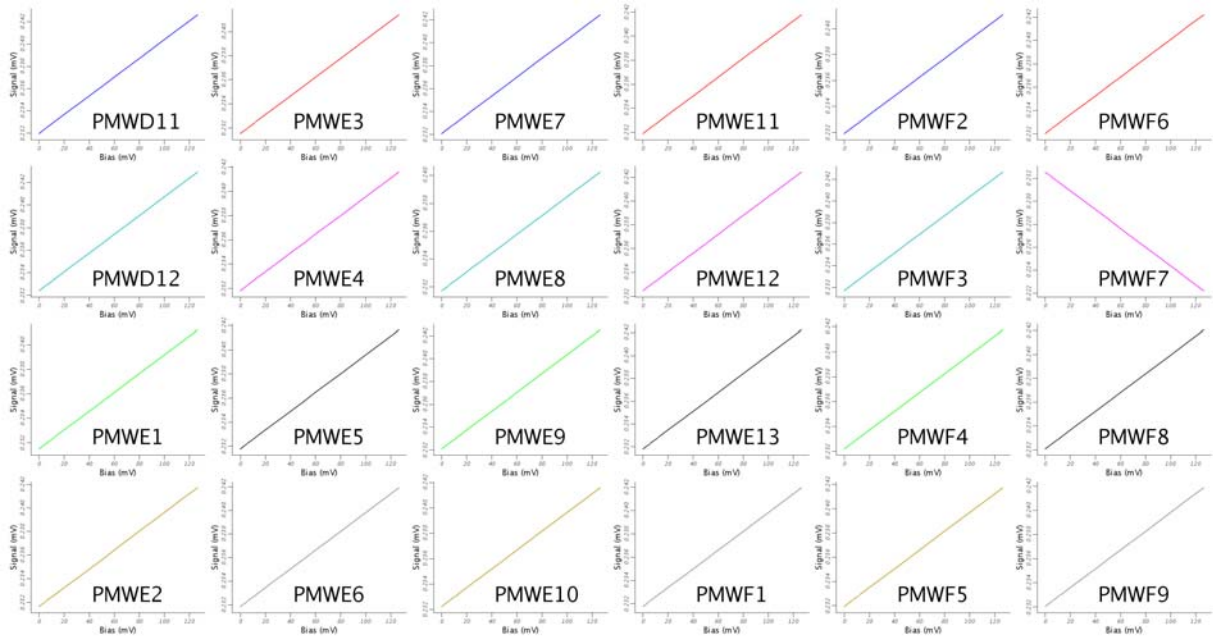


Figure 9. PMW Detectors (3)

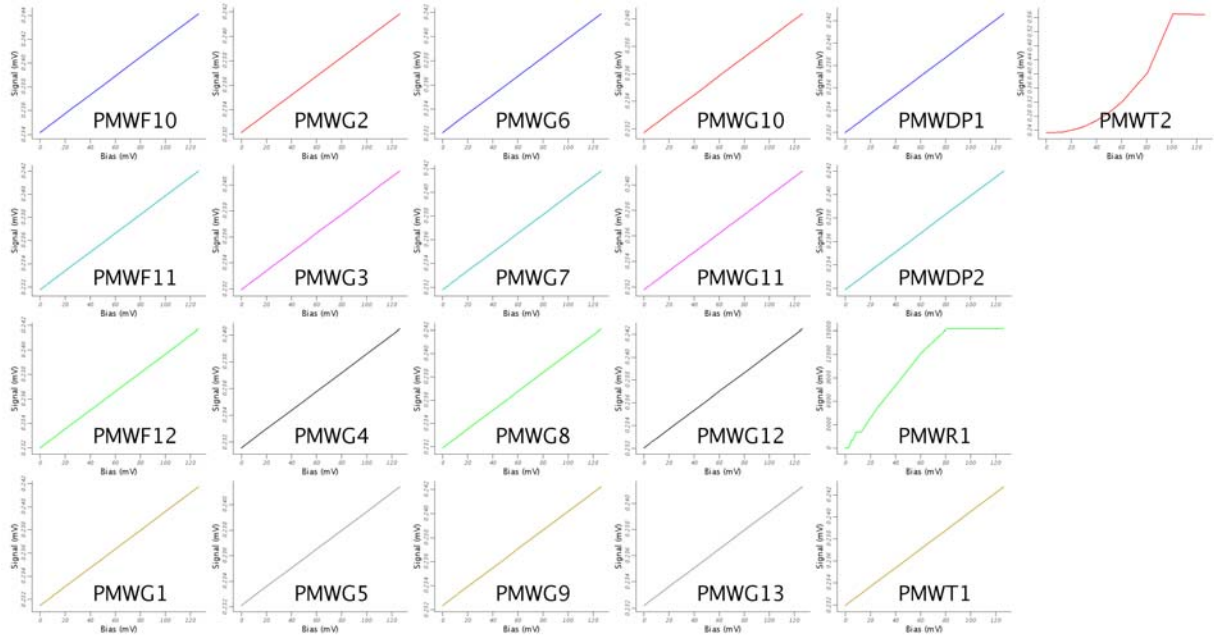


Figure 10. PMW Detectors (4)

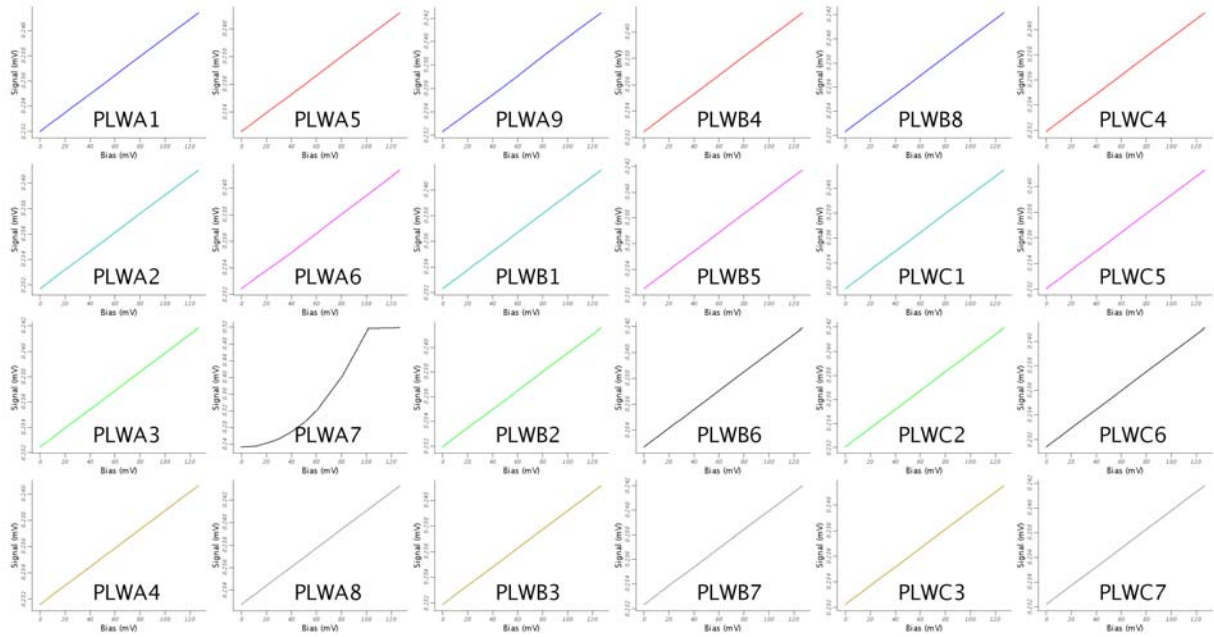


Figure 11. PLW Detectors (1)

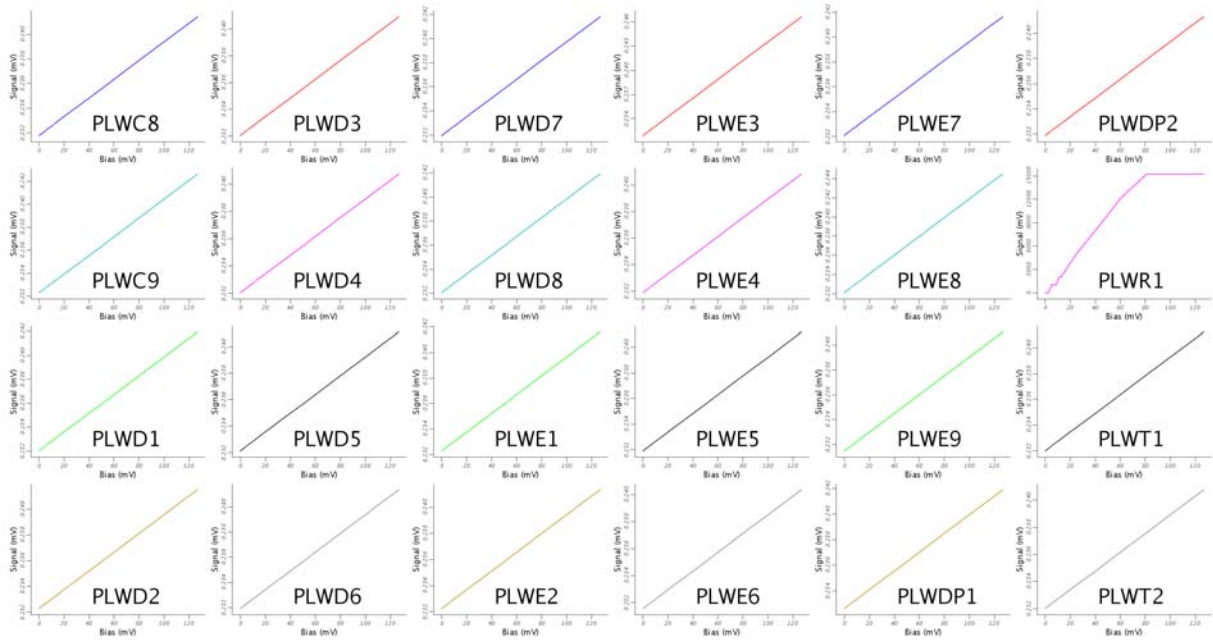


Figure 12. PLW Detectors (2)

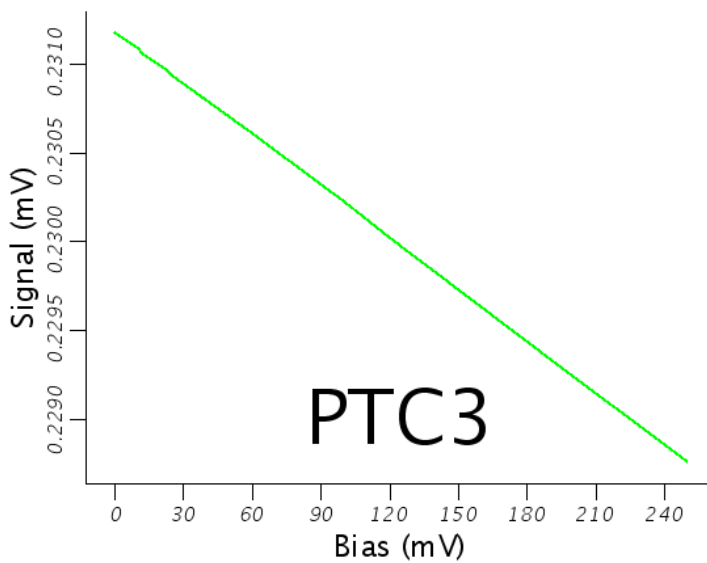
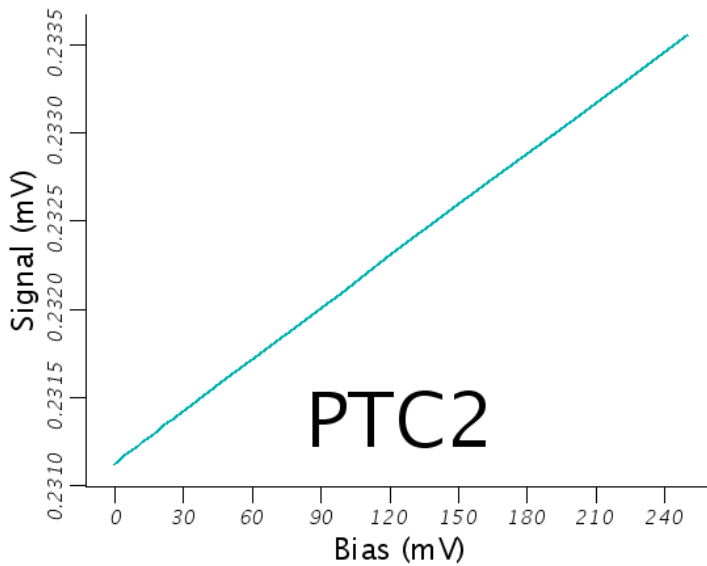
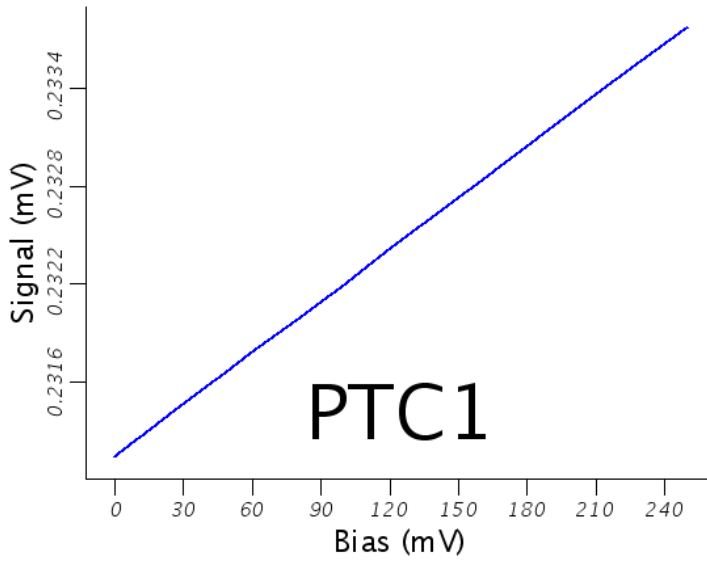


Figure 13. PTC Detectors (1)

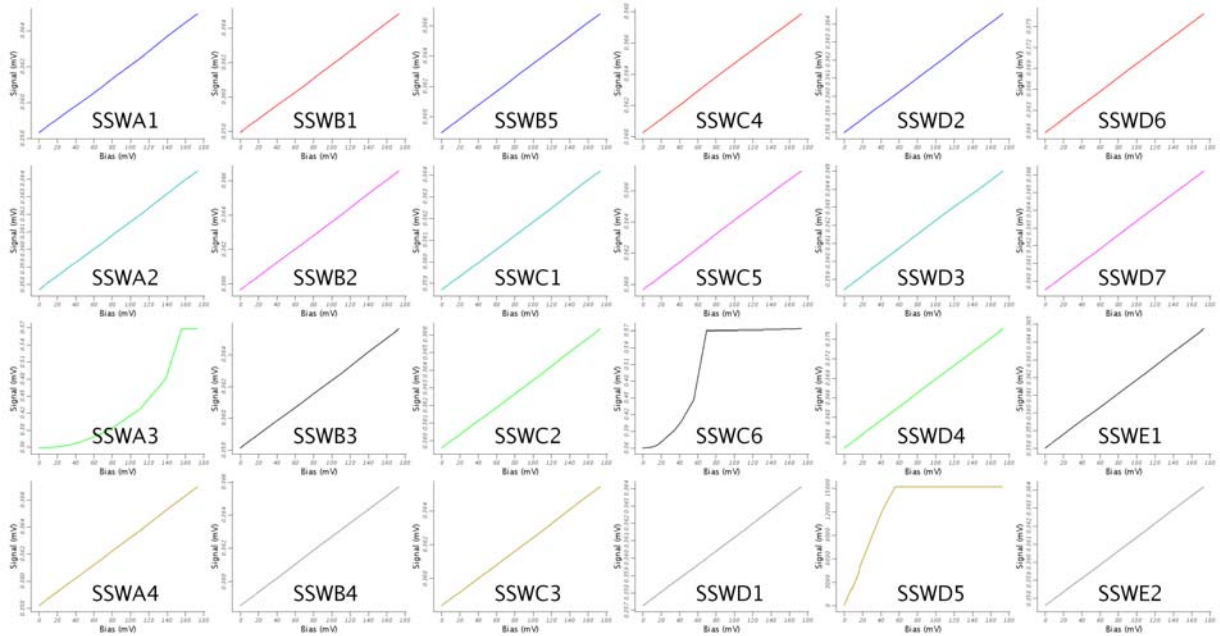


Figure 14. SSW Detectors (1)

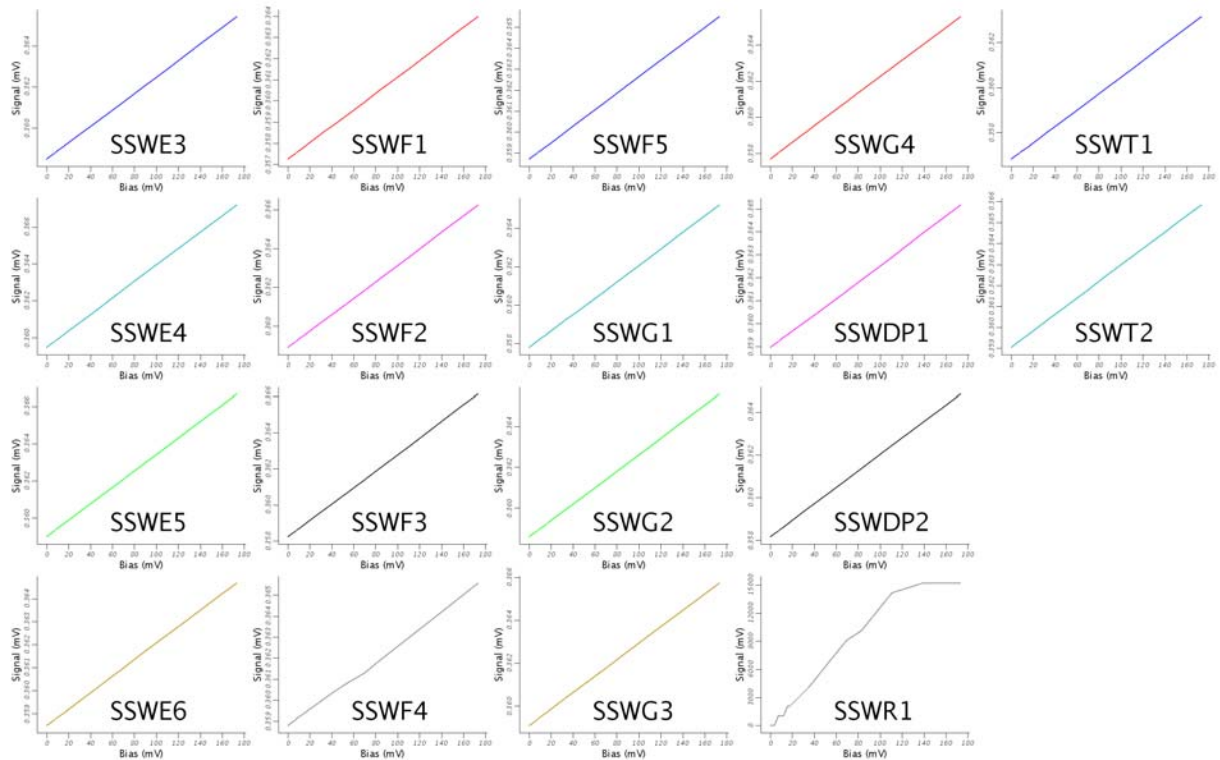


Figure 15. SSW Detectors (2)

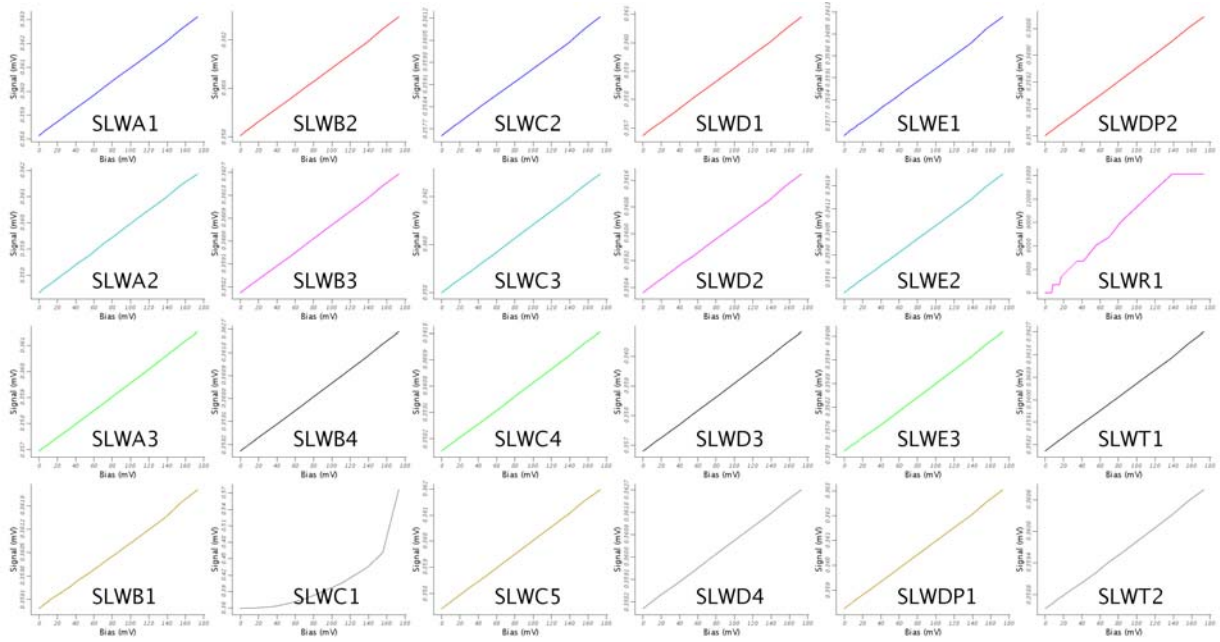


Figure 16. SLW Detectors (1)